

SINCE 1889



Program Type Low Temperature Incubator/ Constant Temperature Incubator

Model: INC822C

- First Edition -

- Thank you for purchasing " Program Type Low Temperature Incubator/Constant Temperature, INC Series " of Yamato Scientific Co., Ltd.
- To use this unit properly, read this "Instruction Manual" thoroughly before using this unit. Keep this instruction manual around this unit for referring at anytime.



WARNING!:

Carefully read and thoroughly understand the important warning items described in this manual before using this unit.

Yamato Scientific Co.,Ltd.

1. Safety precautions	1
Explanation of pictograms	1
List of symbols	2
Warning · Cautions	3
2. Before operating the unit	4
Precautions when installing the unit.....	4
Installation method and precautions	8
Lower stage bath Defrost in Refrigerator	10
3. Names and functions of parts	11
Main unit.....	11
Lower stage bath Operation panel.....	12
Lower stage bath Description of characters	13
Upper stage bath Operation panel.....	14
Upper stage bath Description of characters.....	15
4-1. Operating procedures (lower stage)	16
Lower stage bath List of operation modes and functions	16
Lower stage bath Overheat preventive device setting	20
Lower stage bath Operating procedures (fixed value operation)	21
Lower stage bath Operating procedures (Quick auto stop operation)	22
Lower stage bath Operating procedures (auto stop operation)	23
Lower stage bath Operating procedures (auto start fixed value running)	25
Lower stage bath Operating procedures (auto start program running)	27
Lower stage bath Operating procedures (making a program)	29
Lower stage bath Program preparation sheet.....	34
Lower stage bath Useful functions (calibration offset function)	36
Lower stage bath Useful functions (lock function)	37
Lower stage bath Useful functions (Defrosting function)	38
4-2. Operating procedures (upper stage)	39
Upper stage bath List of operation modes and functions	39
Upper stage bath Overheat preventive device setting.....	42
Upper stage bath Operating procedures (fixed value operation)	43
Upper stage bath Operating procedures (Quick auto stop operation)	44
Upper stage bath Operating procedures (auto stop operation)	45
Upper stage bath Operating procedures (auto start operation)	47
Upper stage bath Useful functions (calibration offset function)	49
Upper stage bath Useful functions (lock function)	50
5. Handling precautions	51
6. Maintenance	53
Daily inspection/maintenance	53
7. When the unit is not to be used for a long time or when disposing	54
8. When a trouble occurs.....	55
Safety devices and error codes.....	55
Safety units and error codes	56

9. After sales service and warranty..... 57
 When requesting a repair 57
10. Specifications..... 58
11. Wiring diagram..... 59
12. Replacement part table..... 60
13. List of dangerous materials..... 61
14. Standard installation manual..... 62

1. Safety precautions

Explanation of pictograms

About pictograms

A variety of pictograms are indicated in this operating instruction and on products for safe operation. Possible results from improper operation ignoring them are as follows.

Be sure to fully understand the descriptions below before proceeding to the text.

 **Warning** Indicates a situation which may result in death or serious injury (Note 1.)

 **Caution** Indicates a situation which may result in minor injury (Note 2) and property damages (Note 3.)

(Note 1) Serious injury means a wound, an electrical shock, a bone fracture or intoxication that may leave after effects or require hospitalization or outpatient visits for a long time.

(Note 2) Minor injury means a wound or an electrical shock that does not require hospitalization or outpatient visits for a long time.

(Note 3) Property damage means damage to facilities, devices and buildings or other properties.

Meanings of pictograms



This pictogram indicates a matter that encourages the user to adhere to warning ("caution" included).
Specific description of warning is indicated near this pictogram.



This pictogram indicates prohibitions
Specific prohibition is indicated near this pictogram.



This pictogram indicates matters that the user must perform
Specific instruction is indicated near this pictogram.

1. Safety precautions

List of symbols

Warning



General warnings



Danger!: High voltage



Danger!: High temperature



Danger!: Moving part



Danger!: Hazard of explosion

Caution



General cautions



Electrical shock!



Burning!



Caution for no liquid heating!



Caution for water leak!



For water only



Poisonous material

Prohibitions



General bans



Fire ban



Do not disassemble



Do not touch

Compulsions



General compulsions



Connect ground wire



Install levelly



Pull out the power plug



Periodical inspection

1. Safety precautions

Warning · Cautions

Warning



Never operate the unit in an atmosphere containing flammable or explosive gas

Never operate the unit in an atmosphere containing flammable or explosive gas. Otherwise, an explosion or a fire may result since the unit is not explosion-proof. See section "13. List of dangerous materials" on page 61.



Be sure to connect the ground wire.

Connect the earth wire to an earthed outlet. When an earthed outlet is not available, use an earthed adaptor and be sure to earth the lead wire for earthing. Otherwise, an electric shock or a fire from electric leakage may result.



Ban on operation when an abnormality occurs

When a smoke or an unusual odor is seen or sensed, immediately turn the power supply OFF. A fire or an electrical shock may result.



Never use electrical power cords bundled.

When these are used bundled, they might overheat causing a fire.



Take care not to damage electrical power cords.

Avoid tightly bend, pull with a strong force or twist to prevent electrical power cords from damaging. A fire or an electrical shock may result.



Never try to disassemble or alter the unit.

Never try to disassemble or alter the unit. A malfunction, a fire or an electrical shock may result.



Caution



When a thunder is heard.

When a thunder is heard, turn the main power off immediately. A malfunction, fire or an electrical shock may result.

2. Before operating the unit

Precautions when installing the unit

1. Carefully select an installation site.




Take special care not to install the unit at a place described below:

- Uneven surfaces or dirty surfaces
- Where flammable gas or corrosive gas exists
- Where the ambient temperature is 35°C or more
- Where temperature changes severely
- Where humidity is high
- Where subject to direct sunlight
- Where vibration is severe




Install this unit at a place with spaces shown below.

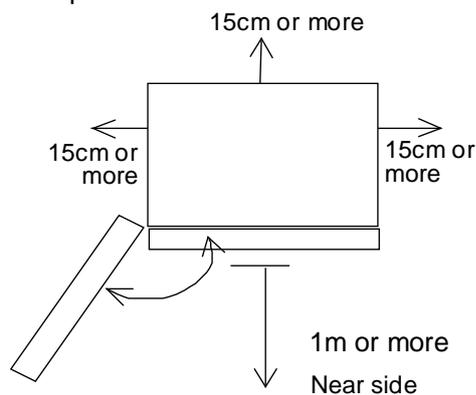

2. Install the unit on a level surface.



Install the unit on a level surface. If the whole bottom surface of the unit does not contact the surface evenly, vibrations or noises may result. This might cause unexpected troubles or malfunctions.

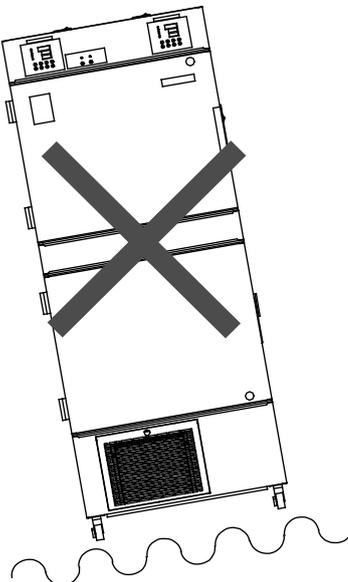

Unit Weight : approx. 160 kg

When lifting the unit for transportation and installation, carefully handle it by at least two people.

3. Installation



The unit might fall down or move by an earthquake or an impact resulting a personal injury. We recommend making safety measures such as to avoid installing the unit at a place other than busy places.

2. Before operating the unit

Precautions when installing the unit

4. Secure sufficient ventilation for the unit.




Do not operate the unit when its side panels and suction port and radiation port on the rear side of the unit are blocked.

Internal temperature of the unit will rise degrading the performance and an accident, a malfunction or a fire may result.

5. Do not operate the unit at such a place that may subject to splash.



Do not operate the unit at such a place that may subject to splash. Liquid entering the inside may cause an accident, a malfunction, an electrical shock or a fire.

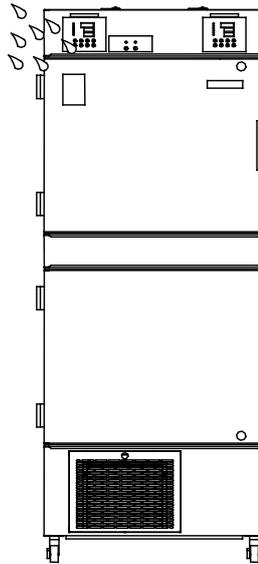


6. Never operate the unit in an atmosphere containing flammable or explosive gas.



Never operate the unit in an atmosphere containing flammable or explosive gas. Since the unit is not explosion-proof, an arc is discharged when switching the ELB "ON" and "OFF" and during operation and a fire or an explosion may result.



See the section "13. List of dangerous materials" on page 61 for flammable and explosive gases.

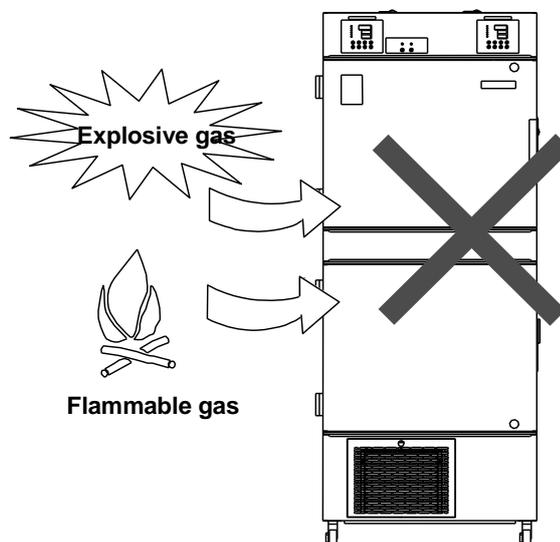

2. Before operating the unit

Precautions when installing the unit

7. Be sure to connect the power plug to the dedicated power distribution panel or a wall outlet.



Use a power distribution panel or a wall outlet that meets the electrical capacity of the unit.

Electrical capacity: AC220V 50Hz 8A

- * When the unit will not start even when you turn the Electric Leakage Breaker to "ON", check for low main voltage or if the unit is connected to the same power supply line as other devices and connect it to another line if necessary.

Avoid connecting too many devices using a branching outlet or extending a wire with a cord reel or heating function and temperature controlling function may degrade due to voltage drop.



Do not connect the unit to any parts or lines other than a correct power supply line such as a gas pipe, a water pipe or a telephone line. Otherwise, an accident or a malfunction may result.

8. Handling of a power cord



Never use electrical power cords bundled. When these are used bundled, they might overheat causing a fire.

Do not convert, forcibly bend, twist or pull the power cord. Otherwise, a fire or an electrical shock may result.

Do not place the power cord under a desk or a chair, or sand between objects to avoid it from being damaged.

Otherwise, a fire or an electrical shock may result.

Do not place the power cord close to a stove or other heat generating device. Sheath of the cord may burn and result in a fire or an electrical shock.



If the power cord should be damaged (exposure of core wire or disconnection), immediately turn the ELB off, turn the power supply off and ask your dealer to replace the cord. If the unit is operated with a damaged power cord, a fire or an electrical shock may result.



Connect the power cord to an appropriate distribution board or wall outlet.

9. Be sure to connect the ground wire.





- When the outlet has no earth terminal, class D earthing work will be necessary. Consult your dealer or one of our sales offices.
- Be sure to connect firmly to the outlet.



We recommend use of a ground type outlet When a bipolar type outlet tap is used

tap

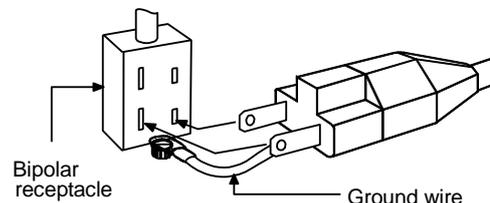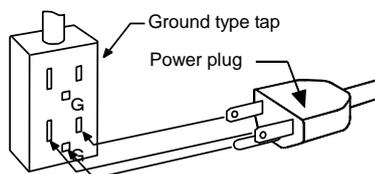

When there is no ground terminal.

In this case, class D grounding work is necessary and please consult your dealer or our nearest sales office.

Insert the ground adaptor included as an option, into a power plug confirming the polarity of the outlet. Connect the grounding wire (green) of the ground adaptor to the ground terminal on the power supply equipment.



Do not connect the grounding wire to any parts or lines other than a correct grounding terminal such as a gas pipe, a water pipe or a telephone line. Otherwise, an accident or a malfunction may result.


2. Before operating the unit

Precautions when installing the unit

11. Do not attempt to alter the unit



The customer shall never attempt to alter the unit. Otherwise a malfunction may result.

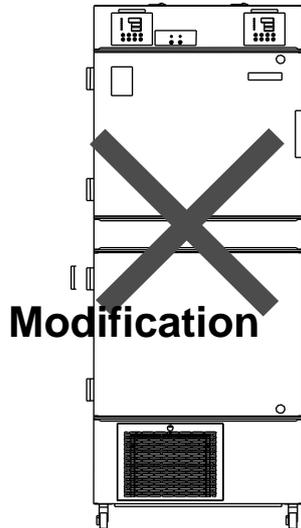


12. Do not put too many specimens.



The withstand load of a shelf board is 15kg when the load is evenly distributed.


Put specimens dispersed.

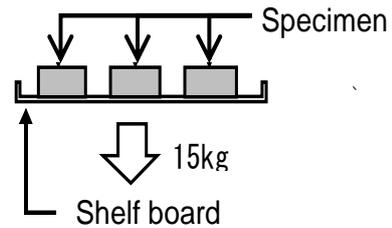

13. Do not set too many specimens.



Too many specimens will prevent correct temperature control. In order to assure temperature precision, be sure to use shelf boards and put specimens dispersed, and secure at least 30% of space inside the bath.

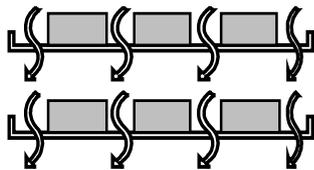

Secure at least 30% of space



Operating the unit with placing the specimen directly on the bottom plate of the internal bath will prevent performance of the product from fully exerting, increase the internal temperature excessively and may cause a malfunction.


Never place a specimen on the bottom plate of the internal bath.

15. Take care during defrosting.



Put a drain pan under the end of the drain hose during defrosting.

Note: Drain pan is not included.

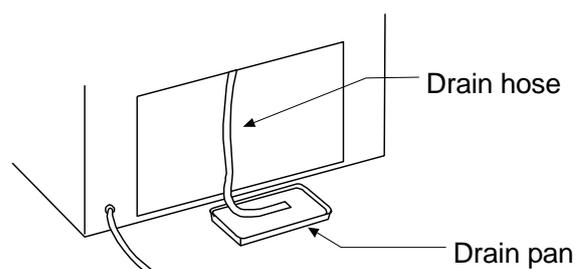


2. Before operating the unit

Installation method and precautions

(1) Transportation of the unit

- When transporting the model INC820, first release lock by pushing stoppers of two caster wheels at the front of the unit as shown in the right diagram. Check that each caster wheel at four points moves smoothly and start transporting the unit.

※ When transporting over a gap, the caster wheels may subject to an excessive shock and be damaged. In such a case, two or more people will be necessary to lift the product over the gap.

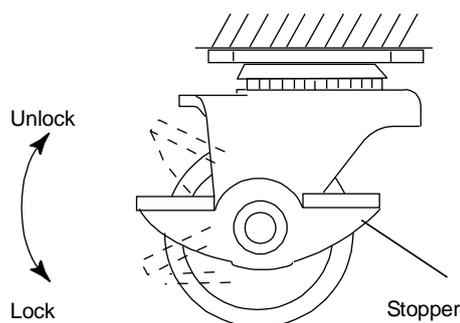

(2) Select an installation site.


Make sure that the each caster wheel at four points rest completely on a flat surface and there is not teetering or inclination, and then lower the caster stoppers and fix them.

(3) Install the shelf boards for the upper stage bath.

- The lowest shelf board for the upper stage bath has been secured with screws at the time of factory shipping.
(The lower stage bath, on whose rear side a heater and other devices are installed, is not fixed.)

Note : Shelf boards differ for the upper and the lower stage baths.

Hole shape of the shelf board for the upper stage bath is round, while that for the lower stage bath board is rectangle.)

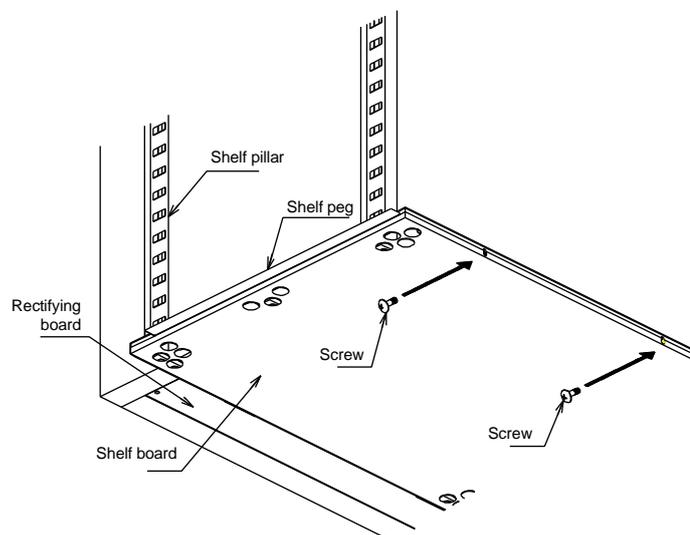


(4) Do not place a specimen on the bottom surface in the internal bath.

- Using the product with a specimen directly placed on the bottom surface in the internal bath may adversely influence on the temperature characteristics. It also may cause corrosion, damages, or rust of the internal bath and burn-out of the specimen or a fire. Never place a specimen on the bottom surface.
- Place a specimen not to touch the wall where sensor or other devices are installed. Put a specimen on the provided shelf board.

2. Before use

Installation method and precautions

- (5) Take care for such specimens as shown below.
- ① Specimen that contains flammable or explosive components.
 - This product is not of an explosion-proof structure. Never attempt to dehydrate or process specimens that contain a flammable or an explosive component.
 - ② Corrosive specimen
 - Take care for handling a corrosive specimen. Although major components are made of SUS304 stainless steel, note that they might corrode with strong acid. Also note that packing (vinyl chloride) may corrode with acid, alkaline, oil, organic solvents, or other substances.
 - ③ Operation with a device with larger heat load introduced.
 - Note that the temperature in the bath may rise when the devices are operated inside the unit.
- (6) About the exhaust port
- There is an exhaust port on the top surface of the main unit.
Adjust the opening according to the moisture content of the specific specimen.

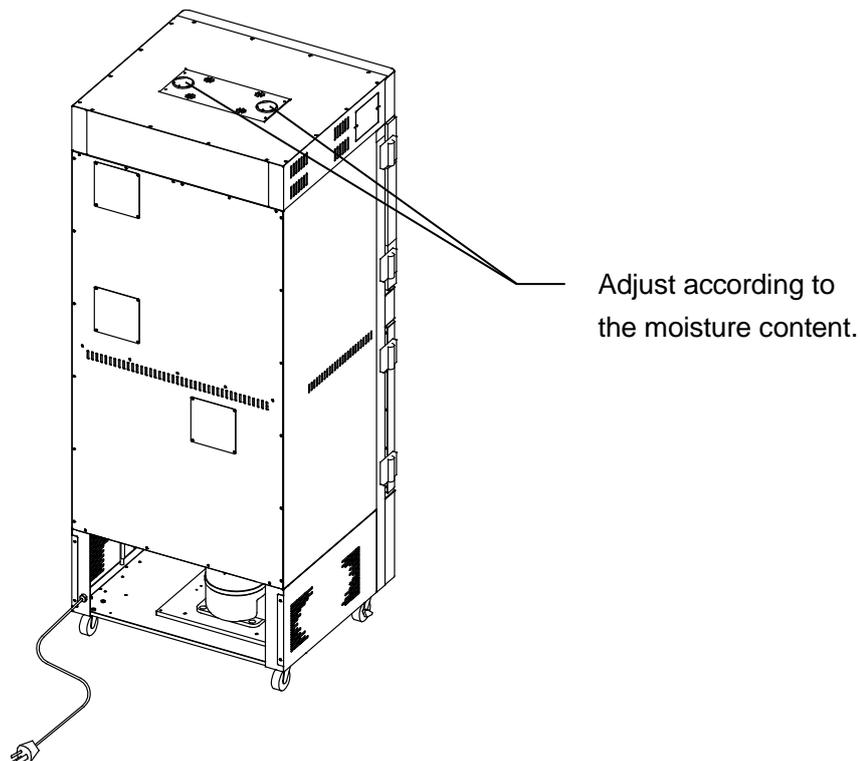

2. Before use

Lower stage bath Defrost in Refrigerator

Once the evaporator of the refrigerator frosts too much, it may lead to reduced refrigeration effect and unable to maintain the set temperature. This product uses the observation window installed inside the chamber to observe the frosting of the evaporator. In addition, the frosting speed also varies according to the following conditions.

- | | |
|---------------------------------------|---|
| (1) Operating temperature |Frost easily when using low temperature |
| (2) External temperature and humidity |Frost easily when using the external temperature and high humidity |
| (3) Sample state in the chamber |Frost easily when using samples containing much water |

Cycle defrost operation (start and stop of operation are automatic)

If need to defrost for a long time, you can set it to cycle defrost operation. Once the defrost operation and stop time is set, it will automatically carry out defrosting at intervals within the set time, repeatedly run and stop. Generally, defrosting can be finished by running defrost operation once a day for about 5 minutes each time, but it still needs to be set according to the operating conditions and the frosting state. When in defrost operation, the temperature control will be temporarily stopped, heater and air supply motor will also be temporarily stopped.

→ See P.34 "Useful functions (defrost)" for details.


Caution

- According to the different operating conditions, during the defrost operation, the temperature in the chamber will rise by about 3°C. Please note that it may influence the samples. In addition, the display temperature may rise by more than 10°C.
- Even if set to cycle defrost, due to the different operating conditions and frosting state, long-term operation will cause more frost. When frost too much, please reduce the cycle defrost time interval **dF o F** or extend the defrosting time **dF o n**. See P.34 "Useful functions (defrost)" for details.


3. Names and functions of parts

Main unit

Front side

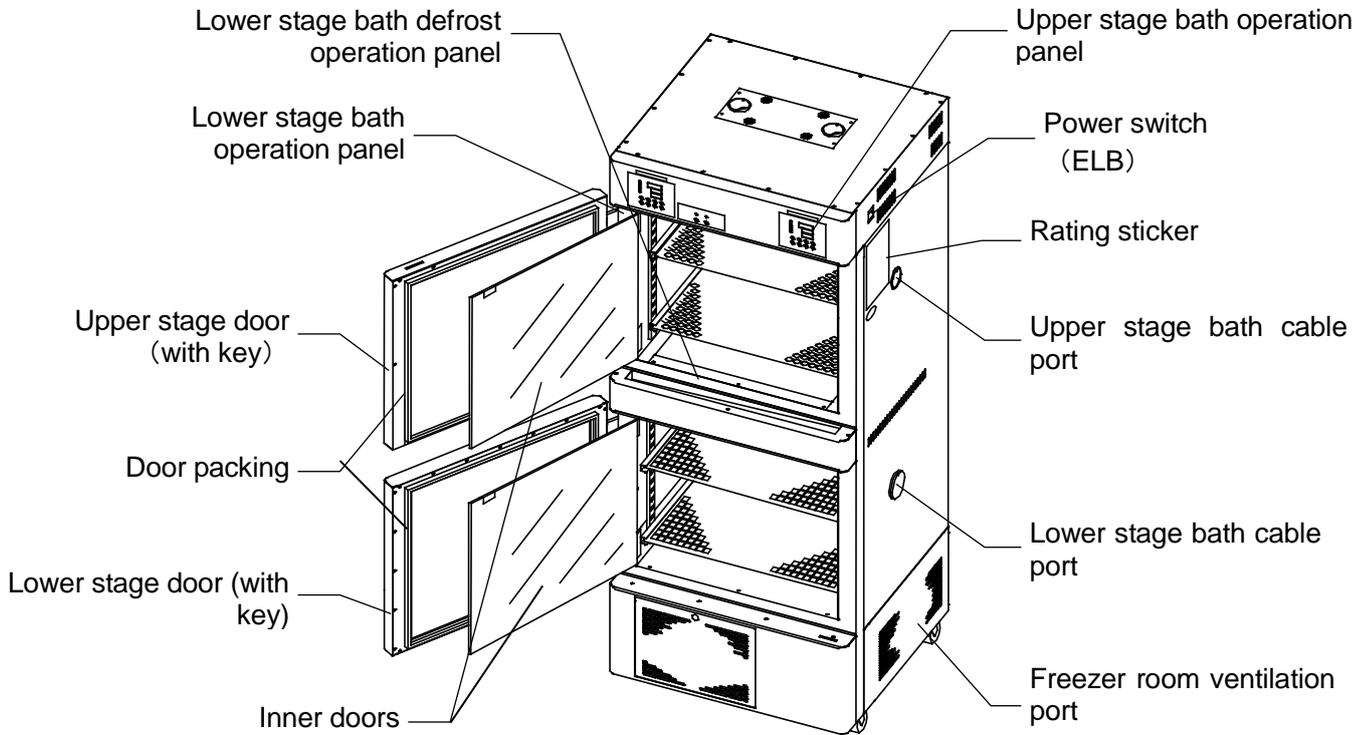


Back side

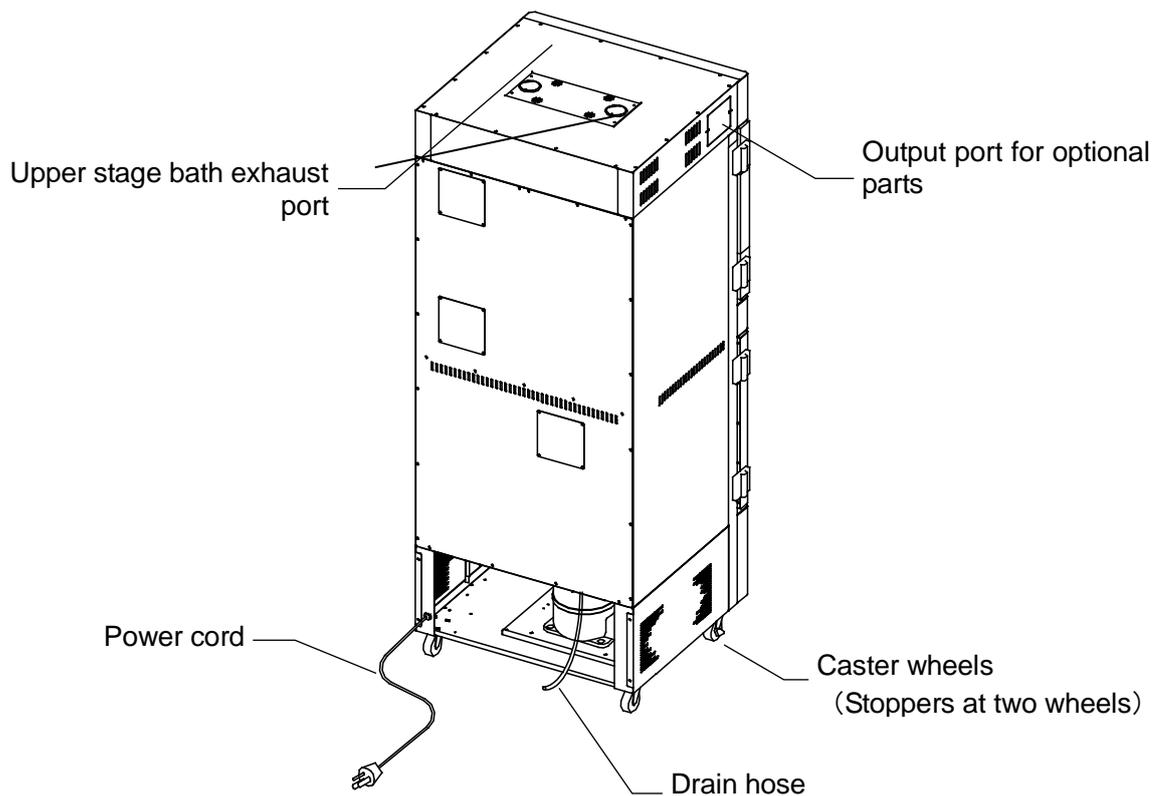

3. Names and functions of parts

Lower stage bath Operation panel

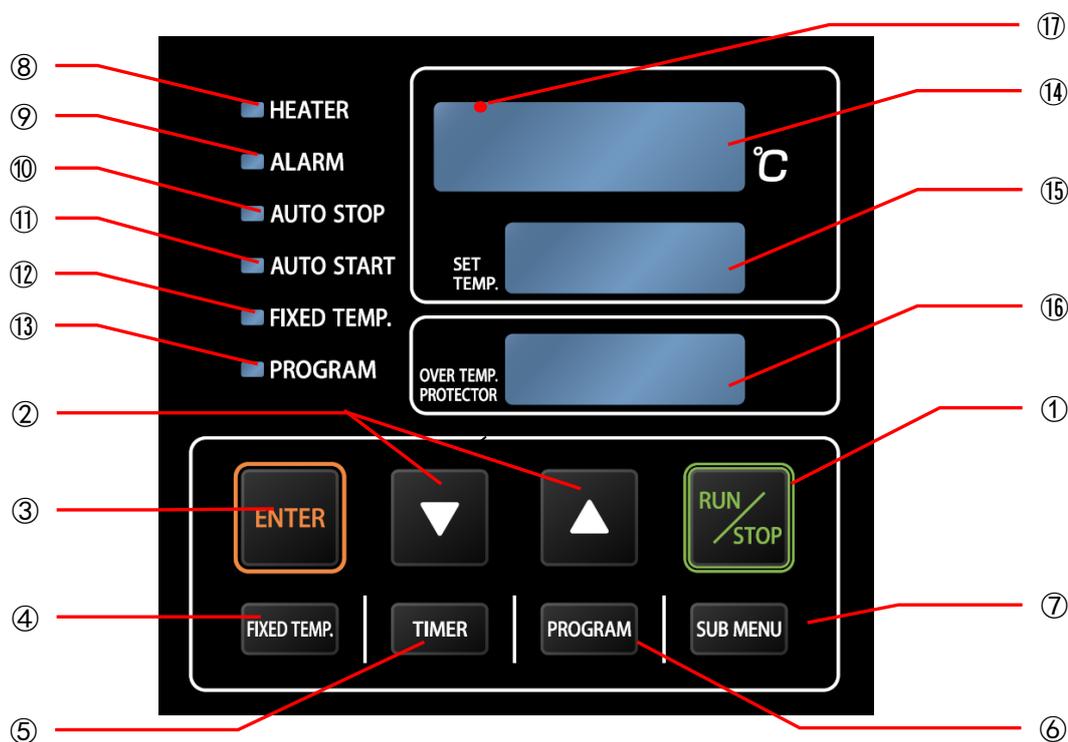

No	Name	Operation/action
①	Start/Stop key	The key is used to start/stop operation.
②	Up/Down keys	These keys are used to select a setting.
③	Enter key	This key is used to determine the selected setting.
④	Fixed-value operation key	This key is used to select the fixed-value operation.
⑤	Timer operation key	Timer operation select key. This key can be used to select the quick auto stop operation, the auto stop operation, or the auto start operation.
⑥	Program key	Program operation select key. You can set programs of 6 patterns of 3 types.
⑦	Sub menu key	The key is used to set for the overheat preventive device temperature, calibration offset temperature, key locks, and the program repeat function.
⑧	Heater lamp	The lamp comes on while power is supplied to the heater.
⑨	Alarm lamp	The buzzer sounds and this lamp comes on when an error occurs.
⑩	Auto stop lamp	This lamp blinks while the quick auto stop timer or the auto stop timer is being set and stays on while either timer is being used.
⑪	Auto start lamp	This lamp blinks while the auto start timer is being set and stays on while it is being used.
⑫	Fixed value operation lamp	This lamp blinks while the fixed value operation is being set and stays on while it is in operation.
⑬	Program operation lamp	This lamp blinks while the program operation is being set and stays on while it is being used.
⑭	Measured temperature display	Displays the measured temperature in the bath, set characters, and alarm information.
⑮	Set temperature display	Displays the set temperature, set temperature, and timer remaining time.
⑯	Overheat preventive device set temperature display	Displays the set temperature of the overheat preventive device.
⑰	Freezer operation lamp	This lamp comes on while power is supplied to the freezer.

3. Names and functions of parts

Lower stage bath Description of characters


Characters used in the model VS4 controller are described below.

Characters	Identifier	Name	Applications
	Fix	Fixed value operation setting mode	You can select the fixed value operation starting function.
	Sv	Temperature setting	This is used to set a temperature.
	Astp	Timer setting mode display	This means the quick auto stop operation and the auto stop operation setting.
	Astr	Timer setting mode display	Automatic start of fixed value running
	Pstr	Timer setting mode display	Automatic start of program running
	Tim	Time setting	This is used to set a time.
	PrG3	Program type select	This is used select one of program types 1 to 3.
	PAt	Program pattern select	This is used to select a program pattern.
	End	Step end	This indicates the total number of steps used. See "End program operation" on P.32.
	Sv-1	Program temperature setting	This is used to set a temperature of each program step. See "Register program (program editing)" on P.31.
	t-1	Program time setting	This is used to set a time of each program step. See "Register program (program editing)" on P.31.
	PS-3	Program repeat return destination select	This is used to select a return destination step during the program repeat operation. See "Use the program repeat function" on P.33.
	Pc-2	Program repeat number setting	This is used to set a number of program repeat operations. See "Use the program repeat function" on P.33.
	cAL	Calibration offset setting	This is used to input a calibration offset temperature. See "Lower stage bath Overheat preventive device setting" on P.20.
	oH	Overheat preventive device temperature setting	This is used to set a temperature for the overheat preventive device. See "Lower stage bath Setting for the overheat preventive device" on P.20.
	Lock	Setting key lock	This locks keys to prevent alteration of setting information. See "lock function" on P.37.
	nG	Setting change disabled	During operation, you cannot change any inputs other than temperature and time settings for the timer and program modes. If you attempt to change them, nG will appear.
	A-DF	Automatic defrost running	During automatic defrost operation, the set temperature displayer  blinks.

※For operation modes and function characters, see "Lower stage bath Operation modes, function setting keys and characters" on P.19.

3. Names and functions of parts

Upper stage bath Operation panel

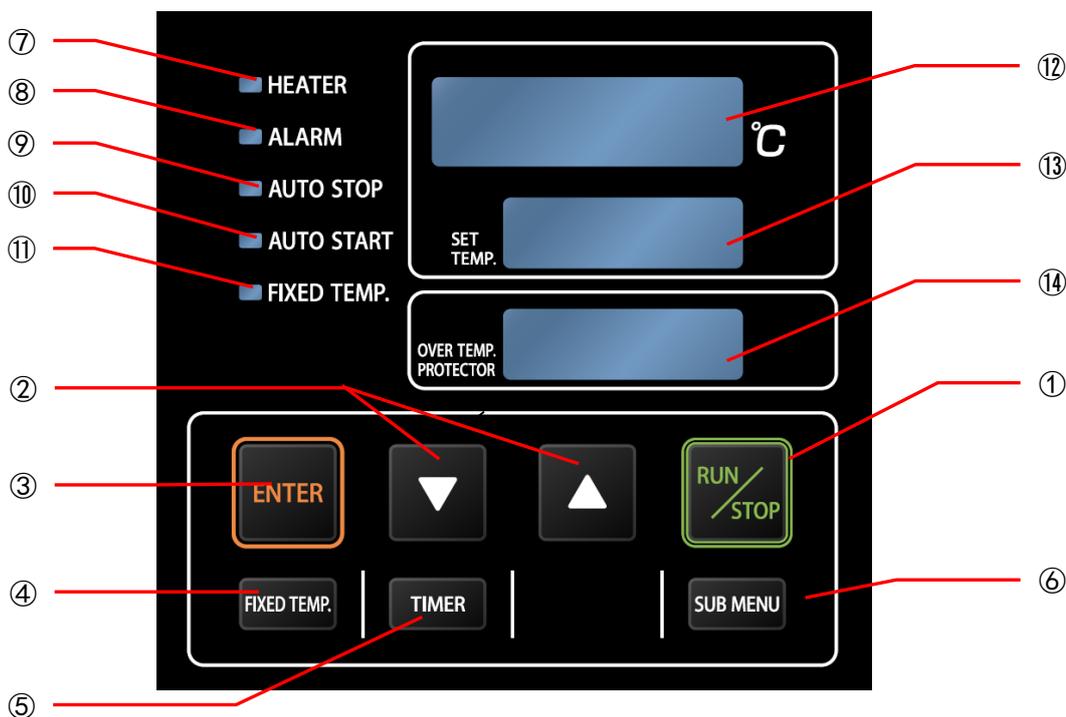


No	Name	Operation/action
①	Start/Stop key	The key is used to start/stop operation.
②	Up/Down keys	These keys are used to select a setting.
③	Enter key	This key is used to determine the selected setting.
④	Fixed-value operation key	This key is used to select the fixed-value operation.
⑤	Timer operation key	Timer operation select key. This key can be used to select the quick auto stop operation, the auto stop operation, or the auto start operation.
⑥	Sub menu key	The key is used to set for the overheat preventive device temperature, calibration offset temperature, key locks, and the program repeat function.
⑦	Heater lamp	The lamp comes on while power is supplied to the heater.
⑧	Alarm lamp	The buzzer sounds and this lamp comes on when an error occurs.
⑨	Auto stop lamp	This lamp blinks while the quick auto stop timer or the auto stop timer is being set and stays on while either timer is being used.
⑩	Auto start lamp	This lamp blinks while the auto start timer is being set and stays on while it is being used.
⑪	Fixed value operation lamp	This lamp blinks while the fixed value operation is being set and stays on while it is in operation.
⑫	Measured temperature display	Displays the measured temperature in the bath, set characters, and alarm information.
⑬	Set temperature display	Displays the set temperature, set temperature, and timer remaining time.
⑭	Overheat preventive device set temperature display	Displays the set temperature of the overheat preventive device.

3. Names and functions of parts

Upper stage bath Description of characters

Characters used in the model VS3 controller are described below.

Characters	Identifier	Name	Applications
	FiX	Fixed value operation setting	This is used for the fixed value operation setting.
	Sv	Temperature setting	This is used to set a temperature.
	AStP	Auto stop setting	This is used for the auto stop operation setting.
	AStr	Auto start setting	This is used for the auto start operation setting.
	tim	Time setting	This is used to set a time.
	End	Time up	It displays the time when the timer operation is completed. See P.44 and 45.
	cAL	Calibration offset setting	This is used to input a calibration offset temperature. See "Upper stage bath Overheat preventive device setting" on P.42.
	oH	Overheat preventive temperature setting	This is used to set a temperature for the overheat preventive device. See "Upper stage bath Overheat preventive device setting" on P.42.
	Lock	Setting key lock	This locks keys to prevent alteration of setting information. See "lock function" on P.37.
	nG	Setting change disabled	During operation, you cannot change any inputs other than temperature and time setting for the timer and modes. If you attempt to change them, nG will appear.

※For operation modes and function characters, see "Upper stage bath Operation modes, function setting keys, and characters" on P.41.

4-1. Operating procedures (lower stage)

Lower stage bath List of operation modes and functions

Operation modes of the unit are as follows.

No.	Name	Description	Page
1	Fixed value operation	<p>Pressing the Fixed temp key brings you to the fixed value operation setting mode.</p> <p>Pressing the Fixed temp key again brings you to the temperature setting mode.</p> <p>Set a temperature with the ▼▲ keys.</p> <p>Press the Start/Stop key to start operation and press the Start/Stop key again to stop.</p>	P.21
2	Quick auto stop operation	<p>This mode is used when you “want to stop operation currently in session automatically after several hours”.</p> <p>You can set time until the operation stop by pressing the Timer key during fixed value operation.</p> <p>Set a time with the ▼▲ keys.</p> <p>Pressing the Start/Stop key will start quick auto stop operation and the timer will activate in the middle of the operation and automatically stop operation after set time.</p>	P.22
3	Auto stop operation	<p>This mode is used when you “want to stop operation automatically before setting fixed value operation”.</p> <p>Press the TIMER key one time at a time until the set temperature display flashes to show R S t P</p> <p>You can set the set temperature “SV” by pressing the Enter key.</p> <p>You can set operation time “tim” by pressing the Enter key again.</p> <p>Pressing the Start/Stop key will start auto stop operation.</p>	P.23
4	Automatic start of fixed value running	<p>This mode is used when you “want to start operation automatically after certain time after power on”.</p> <p>Press the TIMER key one time at a time until the set temperature display flashes to show R S t r</p> <p>You can set the set temperature “SV” by pressing the Enter key.</p> <p>You can set operation time “tim” by pressing the Enter key again.</p> <p>Pressing the Start/Stop key will start auto start fixed value running.</p>	P.25
5	Automatic start of program running	<p>This mode is used when you “want to start operation automatically after certain time after power on”.</p> <p>Press the TIMER key one time at a time until the set temperature display flashes to show P S t r</p> <p>You can set the set program number P r o G by pressing the Enter key.</p> <p>Pressing the Start/Stop key will start auto start program running.</p>	P.27

4-1. Operating procedures (lower stage)

Lower stage bath List of operation modes and functions

Operation modes of the unit are as follows.

No.	Name	Description	Page
6	Program operation	<p>This mode is used when you want to raise or lower the temperature according to the set temperature and time.</p> <p>Press the Program key to display "PrG1".</p> <p>Press the Program key again to select a program mode you want.</p> <p>Press the Enter key to select the pattern "PAT" you want.</p> <p>Press the Enter key to display "End". Then enter the number of patterns to use.</p> <p>Then enter temperature "SV-n" of each pattern and time "t-n" of each pattern serially.</p>	P.29
※You cannot change the operation mode while the unit is in operation. First stop operation before trying to change the mode.			

4-1. Operating procedures (lower stage)

Lower stage bath List of operation modes and functions


Operation functions of the unit are as follows.

No.	Name	Description	Page
1	Overheat prevention function	<p>Automatic overheat prevention function :</p> <p>The function has been set to activate automatically (automatic recovery) at the increase of 6°C when the temperature in the bath has risen linked to the set temperature of the unit.</p> <p>Overheat preventive device :</p> <p>Although the unit shares the power supply, the display unit, and the key input assembly with the controller, it also has an independent temperature measurement circuit, the CPU, the sensors and the output circuit and is able to set any temperature you want on the control panel.</p> <p>If the overheat preventive unit has activated, the unit will stop and will not recover until the power switch is turned on again. (Manual recovery)</p>	P. 20
2	Calibration offset function	<p>The calibration offset function compensates any difference between the target temperature in the bath and the controller controlled temperature (sensor temperature).</p> <p>You can apply compensation to the plus or minus side over the entire temperature range of the unit.</p>	P. 36
3	Overheat prevention temperature compensation function	When you compensate the temperature for the controller in section 2, the temperature of the overheat preventive device will be compensated automatically.	—
4	Power failure compensation function	When a power failure occurs in the middle of operation, this function is used to start operation at the status immediately before power failure.	—
5	Setting lock function	<p>This function is used to lock a set operation mode.</p> <p>You can set or cancel this function with the Sub menu key.</p>	P. 37
6	Setting cycle defrost	<p>Set the cycle defrost OFF interval time.</p> <p>Set the cycle defrost ON running time.</p>	P.38

4-1. Operating procedures (lower stage)

Lower stage bath Operation modes, function setting keys, and characters

Key operations and characters shown below are used for setting an operation mode and a function.

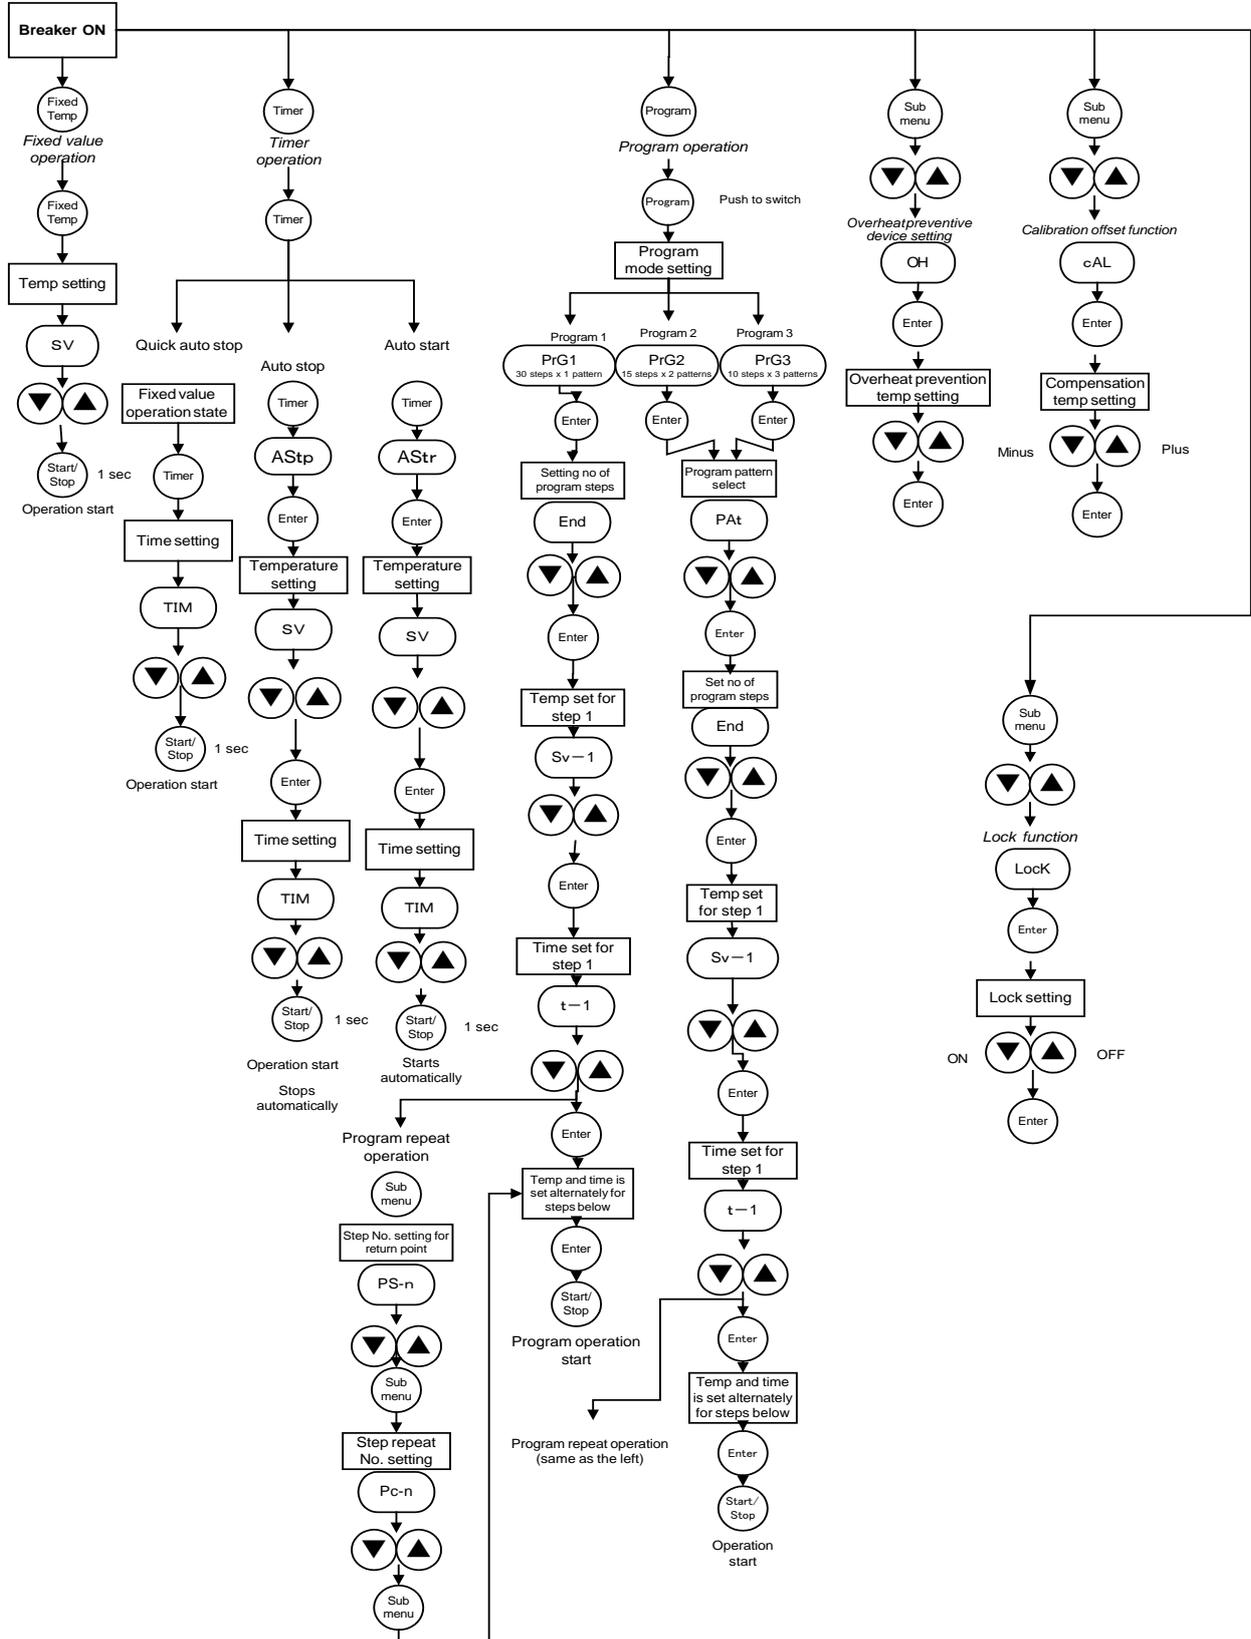

4-1. Operating procedures (lower stage)

Lower stage bath Overheat preventive device setting

The safety units for prevention of overheat includes the power supply, the display, and the key input assembly shared with the controller in addition to the automatic overheat prevention function (automatic recovery) of the controller as well as an overheat prevention device (manual recovery) comprising of the independent temperature measurement circuit, the CPU, and the sensors, and the output circuit, thus establishing dual safety measures.

The overheat prevention device does not aim to protect the specimen but to prevent overheat of devices. This cannot prevent accidents from use of an explosive or a flammable substance.

Temperature setting range and functions

The unit has dual overheat preventive functions. One function is included in the controller and has been set at the time of factory shipping to automatically activate at the temperature 6°C higher than the set temperature of the temperature controller (The heater repeats ON/OFF at a temperature 6°C higher than the setting.)

The other function is integrated with the controller and is set by operating the keys on the controller.



This setting adds the second overheat prevention function.

The temperature setting range of the overheat preventive device integrated with the controller is from 0°C to 105°C.

If the temperature in the bath keeps rising above the controller set temperature and reaches the set temperature of the overheat preventive device, the circuit will be shut off, Er 19 will blink on the controller screen, and the buzzer continues sounding.

Once this overheat preventive device is activated, it holds that status until power is reset and Er19 will not be released.

How to set a temperature

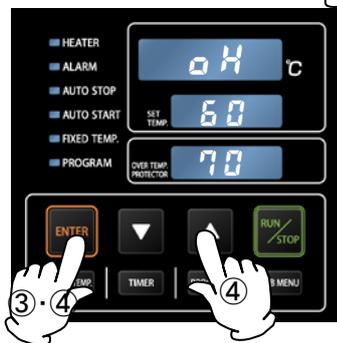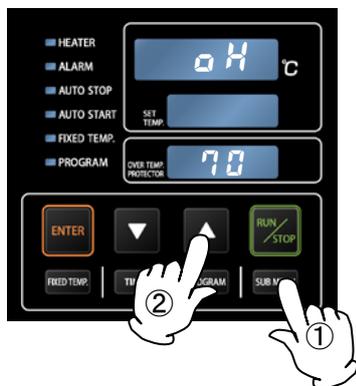

1. Turning power on (Turn the ELB ON)

When you turn power on, the initial values will be displayed for about four seconds, the screen will change to the initial setting screen and each display shows the current temperature in the bath, the operation mode characters, and the overheat prevention set temperature.

2. Setting the overheat prevention temperature

- ① Press the **Sub menu** key.
- ② Press the **▼▲** keys to select the overheat prevention setting characters **OH** on the measured temperature display.
- ③ Pressing the **Enter** key will make the current set temperature blink on the set temperature display.

Caution : Normally, set a temperature higher by 10°C or more than the set temperature on the controller to prevent a malfunction. However, please set it at a temperature that is 15°C or more higher when you drive the defrosting.

- ④ When you have set a temperature you want with the **▼▲** keys, press the **Enter** key to complete setting.

⚠ Caution

- ① Rough guidelines for the set temperature are “the highest temperature possible for the unit +10°C” or “set temperature +10°C” and if malfunctions occur at these settings, add about 5°C to the setting.
- ② The temperature setting range of the overheat preventive device is from 0°C to 70°C. Be sure to set the overheat prevention threshold temperature. Otherwise, devices may not operate properly, the overheat preventive device may activate in the middle of increase of the temperature in the bath, or a fire or other unexpected accidents may result.

The temperature is set at 70°C at factory shipping.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (fixed value operation)

How to conduct fixed value operation



1. Turning power on (Turn ELB ON)

When you turn power on, the software version will be displayed for about four seconds, the screen will change to the initial setting screen and each display shows the current temperature in the bath, the operation mode characters, and the overheat prevention set temperature.

- Measured temperature display : Displays the current temperature in the bath
- Set temperature display : Displays the operation mode characters
- Overheat prevention set temperature display : Displays the set temperature of the overheat prevention device

See P.19 for operation mode characters.



2. Selecting an operation mode

Press the **Fixed temp** key to display fixed value operation on the set temperature display.


Display Fix **F.11**.

3. Setting a temperature

① Press the **Fixed temp** key again.

The characters SV **5.0** that indicate temperature setting will appear on the measured temperature display, the current set temperature blinks on the set temperature display, and the fixed value operation lamp blinks.

② Set the temperature you want with the **▼▲** keys.

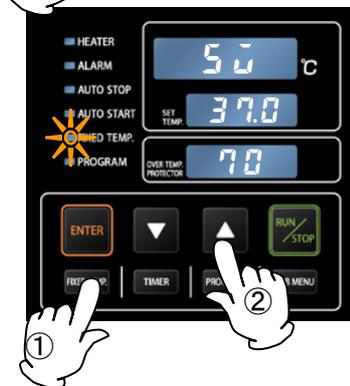

4. Starting operation

Press the **Start/Stop** key for about one second. Operation starts and the fixed value operation lamp will change its status from blinking to on.

5. Stopping operation

Press the **Start/Stop** key for about one second. The fixed value operation lamp will go off and the screen switches to the initial setting screen.



When you want to correct wrong settings or confirm settings

If you made a mistake in setting or when you want to check the setting you have made, press the **Fixed temp** key again and make settings again.

If you want to change the set temperature during operation, press the **Fixed temp** key to enter the setting mode and change the temperature. After change, press the **Enter** key to complete change.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (Quick auto stop operation)

How to perform quick auto stop operation



This operation is used when you “want to stop current fixed value operation automatically after several hours”. Quick auto stop operation allows setting the auto stop timer during operation.

1. Setting a time until stop during fixed value operation

Make sure that the fixed value operation lamp is on to indicate fixed value operation is in session.

Press the **Timer** key.

The characters tim **E n** that indicate the timer appears on the measured temperature display and the current set time blinks on the set temperature display.

Set a time you want with the **▼▲** keys.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.



2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Start the timer operation when the fixed value operation lamp and the auto stop lamp are on.

Timer operation starts when the **Start/Stop** key is pressed.

. Stopping and finishing timer operation

Timer operation will stop automatically at the set time.

The buzzer sounds for five seconds to indicate the timer has stopped. At this time, the characters End **End** that indicate operation complete are displayed on the set temperature display with the fixed value operation lamp and the auto stop lamp are on. Press the **Start/Stop** key for about one second to finish the timer operation mode. The screen will switch to the initial setting screen.


When you want to correct the set temperature, set time, or to confirm settings

When you want to change the set temperature during operation, press the **Fixed temp** key to enter the setting mode and change the temperature. After change, press the **Enter** key to complete change. If you want to change the set time during operation, press the **Timer** key to enter the setting mode and change the time. Note however, that you need to set a time calculated by adding the passed time to the time to add. After change, press the **Start/Stop** key to complete change. You can display the set temperature, the operation mode, and the remaining time on the set temperature display by pressing the **▼** key.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (auto stop operation)

How to perform auto stop operation

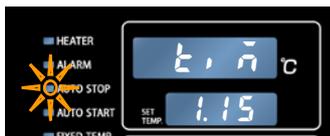

This operation mode is used when “you want to stop fixed value operation automatically after set time since the start”.

1. Setting a stop time

- ① Press the **Timer** key when the initial screen is displayed.
- ② The timer mode used in the previous session will be displayed on the set temperature display. Pressing the **Timer** key again to make a timer mode blink. Press the **Timer** key again to blink the next timer mode. Select the characters Astp **ASTP** that indicate auto stop operation and press the **Enter** key.

The characters Sv **50** that indicate temperature set appear on the set temperature display and the auto stop lamp will blink.

- ③ Press the **▼▲** keys to set the temperature you want.
- ④ Press the **Enter** key. The characters tim **6.0** that indicate the timer on the measured temperature display and the current set time will blink on the set temperature display.
- ⑤ Press the **▼▲** keys to set the time you want.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.



2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Timer operation will start with the auto stop lamp on.

Timer starts when the temperature in the bath (measured temperature) reaches the set temperature.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (auto stop operation)



3. Stopping and finishing timer operation

Timer operation will stop automatically at the set time.

The buzzer sounds for five seconds to indicate that the timer has stopped. At this time, the characters End End that indicate operation complete are displayed on the set temperature display with the fixed value operation lamp and the auto stop lamp are on. Press the Start/Stop key for about one second to finish the timer operation mode. The screen will switch to the initial setting screen.

When you want to correct the set temperature, set time, or to confirm settings

If you want to change the set temperature or the set time during operation, press the Timer key, set a temperature or a time for auto stop operation with the \blacktriangledown / \blacktriangle keys, and then press the Enter key.

Note however, that when you change the setting you need to set a time calculated by adding the passed time to the time to add.

You can press the \blacktriangledown key during operation to display the set temperature, the operation mode, and the remaining time on the set temperature display.

The remaining time display 1.30 indicates counting-down while the dots are blinking and waiting state while the dots stay on (temperature is increasing or decreasing toward the set temperature) and the timer count is stopped.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (auto start fixed value running)

How to perform auto stat operation



Used for "Timing but not running after starting, and entering fixed value operation only after timing arrives." (Delayed operation)

1. Setting a startp time

- ① Press the **Timer** key when the initial screen is displayed.
- ② The timer mode used in the previous session will be displayed on the set temperature display. Pressing the **Timer** key again to make a timer mode blink. Press the **Timer** key again to blink the next timer mode. Select the characters Astr **Astr** that indicate auto start fixed value running and press the **Enter** key.

The characters Sv **50** that indicate temperature set appear on the set temperature display and the auto start lamp will blink.

- ③ Press the **▼▲** keys to set the temperature you want.
- ④ Press the **Enter** key. The characters tim **6.7** that indicate the timer on the measured temperature display and the current set time and autostarat lamp will blink on the set temperature display.
- ⑤ Press the **▼▲** keys to set the time you want.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.



2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Timer operation will start with the auto start lamp on

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (auto start fixed value running)



3. Stopping and finishing timer operation

Operation will start automatically when the set time comes.

Press the **Start/Stop** key for about one second to stop or finish operation. The screen switches to the initial setting screen.

When you want to correct the set temperature, set time, or to confirm settings

If you want to change the set temperature or the set time during operation, press the **Timer** key, set a temperature or a time for auto start fixed value running with the **▼▲** keys, and then press the **Enter** key.

Note however, that when you change the setting you need to set a time calculated by adding the passed time to the time to add.

You can press the **▼** key during operation to display the set temperature, the operation mode, and the remaining time on the set temperature display.

Note that you cannot change them if you have started operation after the auto start time has passed. In this case, stop operation once with the **Start/Start** key and resume setting from the start.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (auto start program running)

How to perform auto stat operation



Used for "Timing but not running after starting, and entering program operation only after timing arrives." (Delayed operation)

1. Setting a startp time

- ① Press the **Timer** key when the initial screen is displayed.
- ② The timer mode used in the previous session will be displayed on the set temperature display. Pressing the **Timer** key again to make a timer mode blink. Press the **Timer** key again to blink the next timer mode. Select the characters pstp **P5tP** that indicate auto start program running and press the **Enter** key.
The characters prog **Prog** that indicate temperature. Setting the temperature display to display the current setting program
- ③ Press the **▼▲** keys to set the program num you want.
- ④ Press the **Enter** key. The characters tim **t.n** that indicate the timer on the measured temperature display and the current set time and autostarat lamp will blink on the set temperature display.
- ⑤ Press the **▼▲** keys to set the time you want.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.




2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Timer operation will start with the auto start lamp on

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (auto start program running)

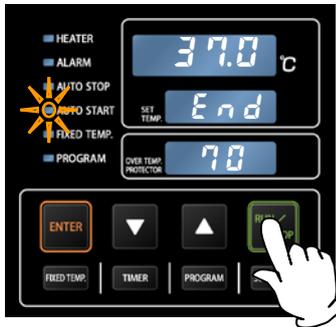

3. Stopping and finishing timer operation

Operation will start automatically when the set time comes.

After the program operation ends, the alarm alarms for about 5 seconds to notify.

The controller is in the operation end prompt state. The automatic start operation indicator light and the program operation indicator light up, and the set temperature display displays the operation end symbol (End), prompting the operator to end the program operation. Note: You are still in running mode at this time.

Press the **Start/Stop** key for about one second to stop or finish operation. The screen switches to the initial setting screen.

When you want to correct the, set time, or to confirm settings

If you want to change the set time during operation, press the **Timer** key, set a time for auto start program running with the **▼▲** keys, and then press the **Enter** key.

Note however, that when you change the setting you need to set a time calculated by adding the passed time to the time to add.


You can press the **▼** key during operation to display the set temperature, the operation mode, and the remaining time on the set temperature display.

Note that you cannot change them if you have started operation after the auto start time has passed. In this case, stop operation once with the **Start/Start** key and resume setting from the start.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (making a program)

Program operation This operation mode is used when “you want to perform operation while increasing and decreasing temperature depending on the time flow”.

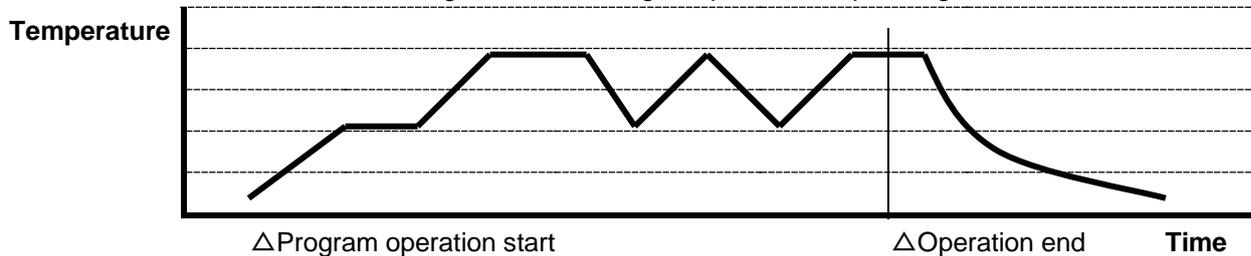

Program types

Up to six program patterns can be stored in memory.

PrG1	You can make one pattern of program up to 30 steps.
PrG2	You can make two patterns of programs up to 15 steps each.
PrG3	
PrG4	
PrG5	You can make three patterns of programs up to 10 steps each.
PrG6	

Before inputting a program

You need to register (input) a program pattern to perform program operation.

- ① Confirm the number of steps, temperature of each step, and time for each step of the prepared program on the program preparation sheet on P. 34 & P. 35 of the instruction manual.
- ② Check the heating or the cooling capacity of the unit. You need to set a temperature within the heating or the cooling capacity of the unit.

For example, when a unit has a capacity for heating or cooling for 3°C for 10 minutes, about 35 minutes will be necessary to decrease or increase the current temperature by 10°C.

Useful functions

You can use the repeat function useful for repeating the same program steps. See “ Operating procedures (program repeat operation)” on P. 33 for how to use the repeat function.

- ① Make sure that the controller has free patterns sufficient for the number of steps you are going to program.
- ② Note however, that you can exclude the number of steps that require free patterns when you use the repeat function above.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (making a program)

Time for increasing or decreasing temperature

Rough time required for increasing or decreasing a temperature is as shown below.

Figures indicate time required for each temperature step. Be sure to perform trial operation and set a correct time because time required for stabilize the temperature reached the setting must be added separately.

Conditions : Room temperature:23°C No load



20°C~50°C : 25 min.

20°C~-10°C : 45 min.

Making a program

A sample program pattern below is used for explanation here.

1. Sample program pattern

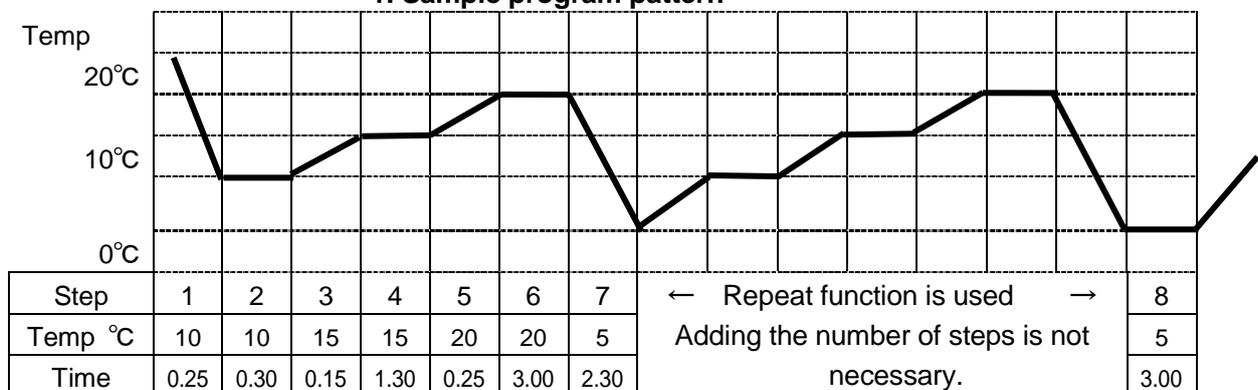

2. Turning power on (Turn ELB ON)

When you turn power on, the initial values will be displayed for about four seconds, the screen will change to the initial setting screen and each display shows the current temperature in the bath, the operation mode characters, and the overheat prevention set temperature.



3. Selecting a program mode and a program pattern

- ① Press the **Program** key.

The program mode used in the previous session will appear on the set temperature display.

Pressing the **Program** key again will blink the program mode.

Pressing the **Program** key again will blink the next program mode.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (making a program)



4. Register program (program editing)

- ① When standby in other mode, press **PROGRAM** key. The set temperature display displays **PrG1**, enter the program mode.
- ② Repeatedly press **PROGRAM** key. The set temperature display will cycle display **PrG1** ~ **PrG8**, select the program you want to edit, press **ENTER** key to confirm.
- ③ The measured temperature display displays **End**, prompts to enter the end segment of the selected program here, and the set temperature display displays the currently specified end segment. The graphic example sets 30, indicating that there are 30 segments in the program. After running the segment 30, the program ends. Use the **▼▲** keys to edit, and the press **ENTER** key to confirm.

※ Note: the maximum number of available program segments is different depending on the program you select. Refer to Page 29 "Program types".

- ④ The measured temperature display displays **50.1** (Sv-1), prompts to enter the set temperature of program segment 1 here. Press the **▼▲** keys to set the required temperature to the set temperature display, press **ENTER** key to confirm. In the graphic example, set according to the program example, the temperature of the first segment is 30.0°C.
- ⑤ The measured temperature display displays **t-1** (t-1), prompts to enter the run time of program segment 1 here. Press the **▼▲** keys to set the required time to the set temperature display, press **ENTER** key to confirm. In the graphic example, set according to the program example, the time of the first segment is 10min.

※ Before setting the time, check the temperature rise/drop limit of the device.

※ Example: for IQ823C, it takes about 25 minutes for the temperature to rise from room temperature to 50°C, which can be considered as 1°C rise per minute. But actually, the higher the temperature, the harder it is to heat up, and the lower the temperature, the harder it is to cool down. Please set a sufficient time.

※ The max. set time for each segment is 999 hours and 50 minutes.

- ⑥ After time setting, press **ENTER** key to confirm, display the set temperature symbol **50.2** of the program segment 2, press **▼▲** keys to set temperature, use the same way to operate the following program segments. Please enter the temperature and time of each segment according to the programming data.
- ⑦ The different method is necessary when program repeat function is used. In this case, after setting the time (t_4 in the example) in the segment where the repeat operation is to be used (segment 7 in the example), press the **SUBMENU** key to enter the repeat function setting mode.

※ For the operation and editing methods of program repeat function, please refer to page 33 "Use the program repeat function".

- ⑧ After setting the temperature and time in the last segment, it will return to the initial screen.

4-1. Operating procedures (lower stage)

Lower stage bath Operating procedures (making a program)



Make sure to check the setting temperature and time by operating the unit without load before performing actual run with samples.

5. Start program operation

Long press the **RUN/STOP** key, the set program starts to operate. Please refer to page 30 "Selecting a program mode and a program pattern" for program selection.

The program lamp lights up, the set temperature display in order of St-1 **St-1** to display the running program segment.

※ Press the **▼** key during operation to confirm the setting temperature and remaining time of each segment on the set temperature display.

6. End program operation

The buzzer will sound for about 5 seconds after operation end.

The controller is in the state of operation end prompt. The program running indicator lamp lights up, and the set temperature display

displays the operation end symbol **End** to prompt the operator that the program operation ends. Note: it is still in operating mode at this time.



Long press the **RUN/STOP** key to stop the operating mode, the indicator lamp goes out and return to the initial screen.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.

When you want to correct wrong settings or to check the setting

When you want to return to the previous step to, for example, check for program errors or to re-check the setting, press the **Fixed temp** key to return the set screen to the previous one.

Each time you press the **Fixed temp** key, you will go back one step.

Note: Be sure to perform these steps in the program setting screen.


About wait operation of program operation

When a program shifts from one step to the next, when the measured temperature has not reached or has exceeded the set temperature even if the set time for the step has passed, the next step will not start. The unit has been set that a step will shift to the next in the range of $\pm 1^{\circ}\text{C}$ to the set temperature.

4-1. Operating procedures (lower stage)


Lower stage bath Operating procedures (making a program)

The program repeat function is used to "run several segments in a program repeatedly". As shown in the figure, although there are 6 segments of the edited program, because the program repeat function is executed at the end of the segment 4, the program jumps to the segment 1 and repeats twice, a total of 14 program segments are actually run, among which segments 1 ~ 4 are executed three times in total.

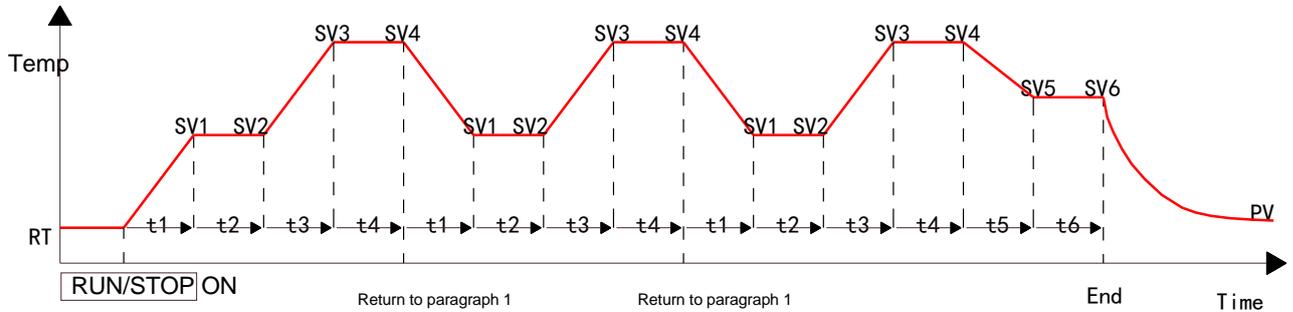

Use the program repeat function


We still use the program example in programming to explain. See P.30 "Making a program".

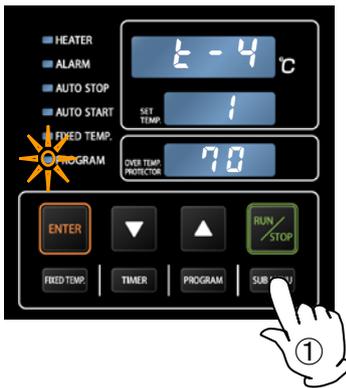

- ① After setting the time of the program segment (segment 4 in the example) that you want to repeat and jump (example t₄), press **SUB MENU** key to enter the repeat function set mode.



- ② The measured temperature displayer displays the symbol **P5_4** 「PS_4」 to prompt to input the address segment to be returned by the program segment 4. It can only be returned to the segment that precedes this segment, so the setting range of the return address **P5_4** is 1~4, use the **▼▲** keys to input the segment number of the return address (on P.30 "Making a program", after the segment 4 ends, it returns to the segment 1, so input 1 at **P5_4**).

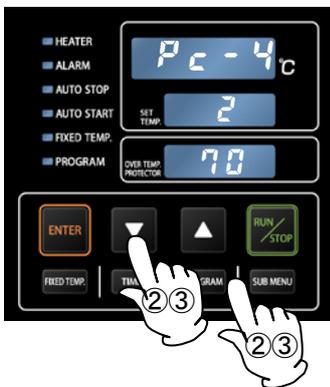

- ③ Press the **SUB MENU** (function key), the measured temperature displayer displays the symbol **Pc_4** 「Pc_4」 to prompt to input the repeat times of the program segment 4 returning to the segment 1. Press the **▼▲** keys to input the times (on P.30 "Making a program", after the segment 4 ends, it returns to the segment 1, which is executed twice, so input 2 at **Pc_4**).

- ④ Press the **SUB MENU** (function key) again, switch to the set temperature screen of the next segment (on P.30 "Making a program", it will move to the display symbol **S0_5**).

- ⑤ The segment 5 and the following program can be edited as normal.

※ The program repeat setting cannot be modified during operation. It must stop the operation, and then follow the above steps to confirm and modify each parameter of program repeat in turn.

4-1. Operating procedures (lower stage)

Lower stage bath Program preparation sheet

Make a copy of this sheet for use.

Registration destination	PrG1 PrG2 PrG3 PrG4 PrG5 PrG6	Management No.	
Name of test		Date y/m/d	
		Prepared by	

Program inputs

	Set temperature (°C)	Set time (time : minute)	Repeat function input (Return to : times)
Step 1		:	:
Step 2		:	:
Step 3		:	:
Step 4		:	:
Step 5		:	:
Step 6		:	:
Step 7		:	:
Step 8		:	:
Step 9		:	:
Step 10		:	:
Step 11		:	:
Step 12		:	:
Step 13		:	:
Step 14		:	:
Step 15		:	:
Step 16		:	:
Step 17		:	:
Step 18		:	:
Step 19		:	:
Step 20		:	:
Step 21		:	:
Step 22		:	:
Step 23		:	:
Step 24		:	:
Step 25		:	:
Step 26		:	:
Step 27		:	:
Step 28		:	:
Step 29		:	:
Step 30		:	:


4-1. Operating procedures (lower stage)

Lower stage bath Useful functions (calibration offset function)

Using the calibration offset function

The calibration offset function compensates any difference between the target in-bath temperature and the control temperature of the controller (sensor temperature). You can apply parallel compensation to the plus or minus side over the entire temperature range of the unit. You can set/cancel this function with the **Sub menu** key.

The offset is set at “0” at the time of factory shipping.

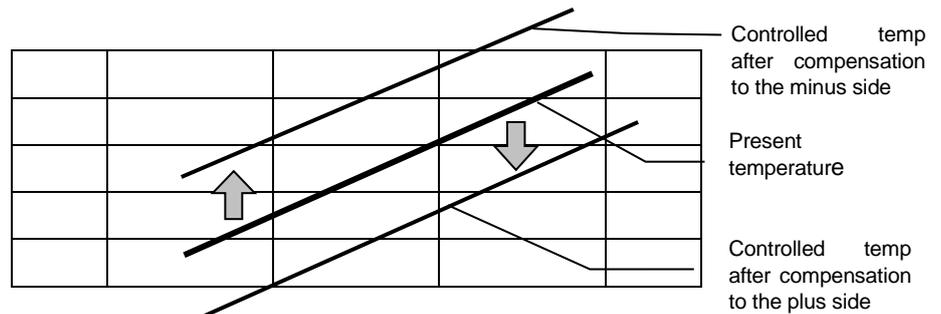

- ① Start operation at the target set temperature and check the in-bath temperature (sample temperature) on a temperature recorder when the temperature is stable.
- ② Check the difference between the set temperature and the in-bath temperature (sample temperature).
- ③ Press the **Sub menu** key and select the character cAL **cAL** that mean calibration offset with the **▼▲** keys and then press the **Enter** key.
- ④ Enter the difference between the set temperature and the in-bath temperature with the **▼▲** keys and press the **Enter** key longer to finish setting.

※ You can set an offset compensation temperature within the range from +99°C to -99°C.

Setting to the - side will decrease the temperature on the measured temp indicator by the compensated temperature and the in-bath temperature will increase by that amount accordingly.

Setting to the + side will increase the temperature on the measured temp indicator by the compensated temperature and the in-bath temperature will decrease by that amount accordingly.

※ Inputting a too large compensation value may cause the actual temperature greatly deviate from the displayed temperature and may be dangerous. So please consult the nearest sales office beforehand.

※ The unit has a two-point compensation function that adjusts offset for the lower temperature region and the high temperature region in addition to the calibration offset function and adjusting temperatures have been set at the time of factory shipping.

※ When validating the temperature indicator, first consult with your nearest sales office or the customer support center.

4-1. Operating procedures (lower stage)

Lower stage bath Useful functions (lock function)

Using the lock function

This function is used to lock the operating status you have set.

This function is set to “off” at factory shipping.



You can set or release this function with the **Sub menu** key.

① Press the **Sub menu** key, select the characters Lock **Lock** that indicate the setting lock with the **▼▲** keys, and then press the **Enter** key.

② "OFF" will appear on the set temperature display. You can lock the settings by setting to "ON" with the **▲** key.

③ To release lock, press the **Sub menu** key, select the characters Lock **Lock** that indicate the setting lock with the **▼▲** keys, and then press the **Enter** key.



Select "OFF" with the **▼** key and then press the **Enter** key to release.





※While the lock function is "ON", any keys other than the **Start/Stop** key and the **Sub menu** key are locked.

4-1. Operating procedures (lower stage)

Lower stage bath Useful functions (Defrosting function)

Select the defrost function

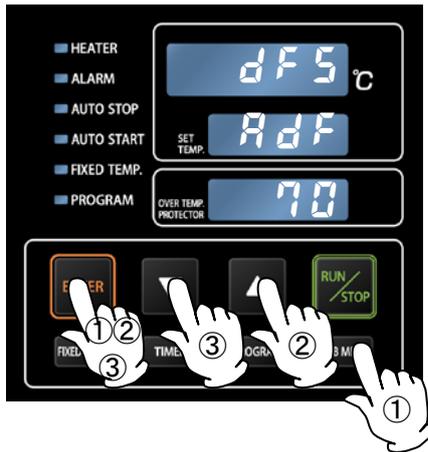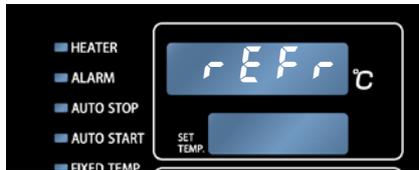

There are three defrost operation functions to select, which are Not use defrost function, Automatic cycle defrost function and Manual defrost function. [Note that this unit does not have the manual defrost function]. After the automatic cycle defrost function is enabled, the time of defrost can be changed, and the interval cycle time of automatic cycle defrost can also be changed.

As per the following steps to make changes:

- ① Press the **SUB MENU** (function key), use the **▼▲** keys to select the symbol **rEFr** (rEFr), press **ENTER** key to confirm.
- ② Repeatedly press **ENTER** key to select the symbol **dFS** (DFS).
- ③ Use the **▼▲** keys to select the defrost function, and press **ENTER** key to confirm.
 - oFF** : Function release (not use defrost function)
 - A dF** : Automatic cycle defrost (factory setting)
 - ñ dF** : Manual defrost (this unit does not have this function)

Set the defrost time



Please follow the above steps to operate, select **dFoN** (dFoN) at the step ②, use the **▼▲** keys to set the duration time of defrost, and then press **ENTER** key to confirm. The setting range is 1 ~ 10 minutes (5mins for factory setting).

Set the stop time of automatic cycle defrost




Please follow the above steps to operate, select **dFoF** (dFoF) at the step ②, use the **▼▲** keys to set the stop time of automatic cycle defrost, and then press **ENTER** key to confirm.

The setting range is 1hr00min ~ 24hrs00min (23hrs55mins for factory setting).

※ Please note that this is to set the stop time of automatic defrost, need to plus the defrost time, which will be a complete defrost cycle time.

Take factory setting as an example, the defrost time is 5mins, the stop time of automatic defrost is 23hrs55mins, then the cycle time of automatic defrost is 24hrs00min. Generally speaking, the automatic defrost runs according to the cycle of OFF→ON→OFF→ON→OFF→ON, OFF time is 23hrs55mins and ON time is 5mins.

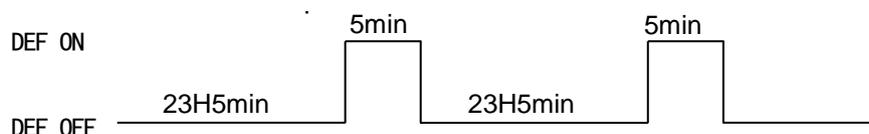

4-2. Operating procedures (upper stage)

Upper stage bath List of operation modes and functions

Operation modes of the unit are as follows.

No.	Name	Description	Page
1	Fixed value operation	<p>Pressing the Fixed temp key brings you to the fixed value operation setting mode.</p> <p>Pressing the Fixed temp key again brings you to the temperature setting mode.</p> <p>Set a temperature with the ▼▲ keys.</p> <p>Press the Start/Stop key to start operation and press the Start/Stop key again to stop.</p>	P. 43
2	Quick auto stop operation	<p>This mode is used when you “want to stop operation currently in session automatically after several hours”.</p> <p>You can set time until the operation stop by pressing the Timer key during fixed value operation.</p> <p>Set a time with the ▼▲ keys.</p> <p>Pressing the Start/Stop key will start quick auto stop operation and the timer will activate in the middle of the operation and automatically stop operation after set time.</p>	P. 44
3	Auto stop operation	<p>This mode is used when you “want to stop operation automatically before setting fixed value operation”.</p> <p>Press the Timer key to display “Astp”.</p> <p>You can set the set temperature “SV” by pressing the Enter key.</p> <p>You can set operation time “tim” by pressing the Enter key again.</p> <p>Pressing the Start/Stop key will start auto stop operation.</p>	P. 45
4	Auto start operation	<p>This mode is used when you “want to start operation automatically after certain time after power on”.</p> <p>Press the Timer key to display “Astr”.</p> <p>You can set the set temperature “SV” by pressing the Enter key.</p> <p>You can set operation time “tim” by pressing the Enter key again.</p> <p>Pressing the Start/Stop key will start auto start operation.</p>	P. 47
<p>※You cannot change the operation mode while the unit is in operation. First stop operation before trying to change the mode.</p>			

4-1. Operating procedures (upper stage)

Upper stage bath List of operation modes and functions


Operation functions of the unit are as follows.

No.	Name	Description	Page
1	Overheat prevention function	<p>Automatic overheat prevention function :</p> <p>The function has been set to activate automatically (automatic recovery) at the increase of 6°C when the temperature in the bath has risen linked to the set temperature of the unit.</p> <p>Overheat preventive device :</p> <p>Although the unit shares the power supply, the display unit, and the key input assembly with the controller, it also has an independent temperature measurement circuit, the CPU, the sensors and the output circuit and is able to set any temperature you want on the control panel.</p> <p>If the overheat preventive unit has activated, the unit will stop and will not recover until the power switch is turned on again. (Manual recovery)</p> <p>You can set or cancel this function with the <u>Sub menu</u> key.</p>	P. 42
2	Calibration offset function	<p>The calibration offset function compensates any difference between the target temperature in the bath and the controller controlled temperature (sensor temperature).</p> <p>You can apply compensation to the plus or minus side over the entire temperature range of the unit.</p> <p>You can set or cancel this function with the <u>Sub menu</u> key.</p>	P. 49
3	Setting lock function	<p>This function is used to lock the operation status you have set.</p> <p>You can set or release this function with the <u>Sub menu</u> key.</p>	P. 50
4	Power failure compensation function	<p>When a power failure occurs in the middle of operation, this function is used to start operation at the status immediately before power failure.</p>	—

4-2. Operating procedures (upper stage)

Upper stage bath Operation modes, function setting keys, and characters

Key operations and characters shown below are used for setting an operation mode and a function.

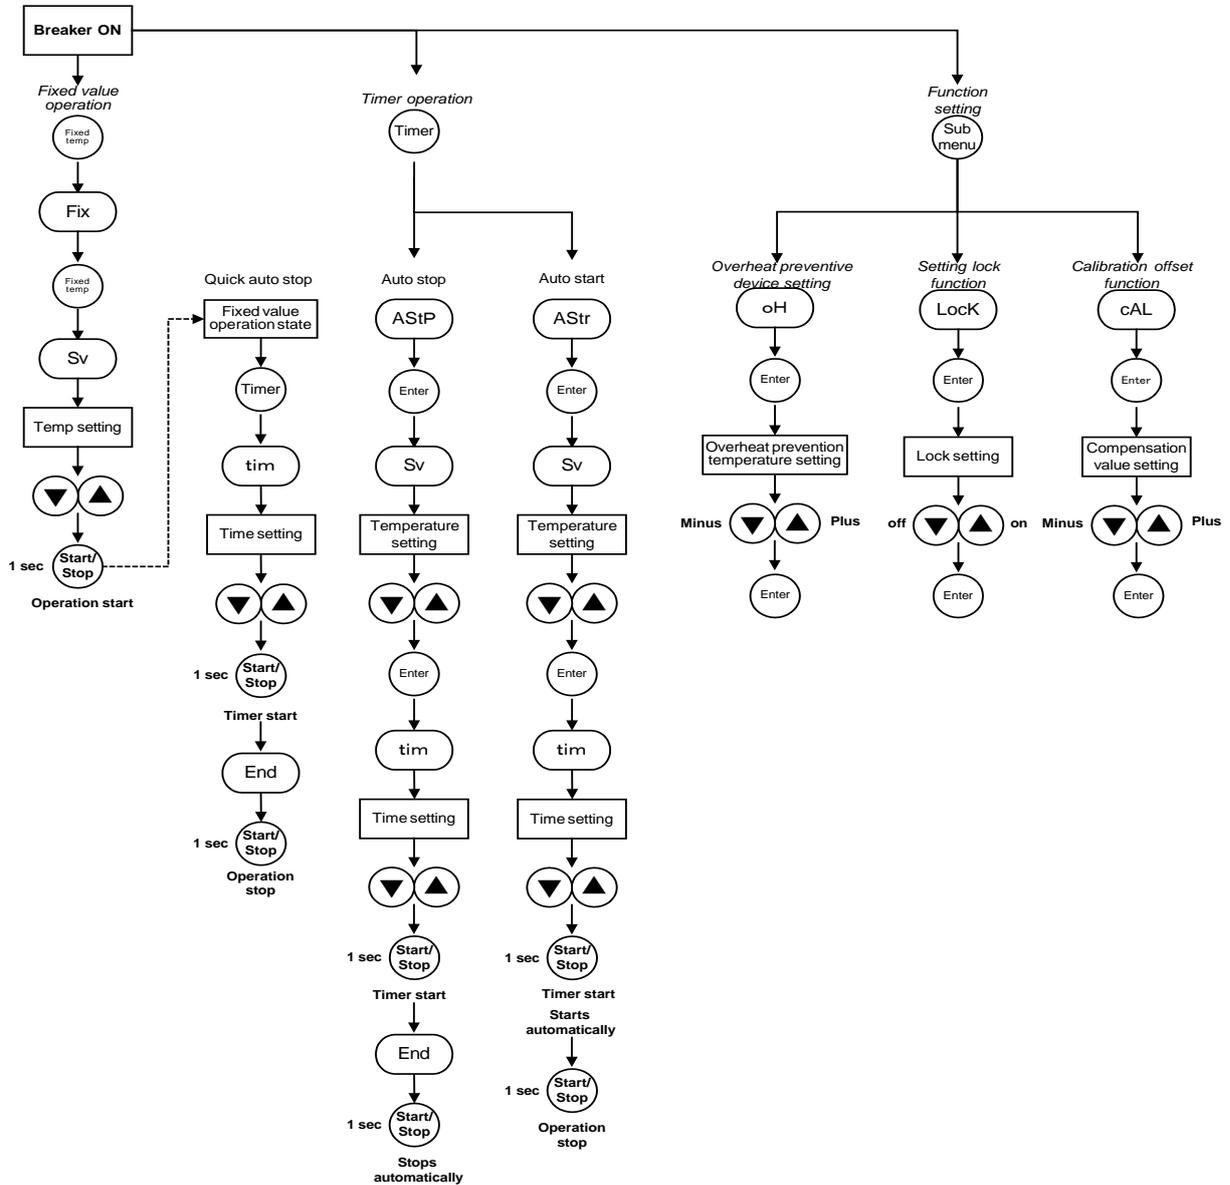

4-2. Operating procedures (upper stage)

Upper stage bath Overheat preventive device setting

The safety units for prevention of overheat includes the power supply, the display, and the key input assembly shared with the controller in addition to the automatic overheat prevention function (automatic recovery) of the controller as well as an overheat prevention device (manual recovery) comprising of the independent temperature measurement circuit, the CPU, and the sensors, and the output circuit, thus establishing dual safety measures.

The overheat prevention device does not aim to protect the specimen but to prevent overheat of devices. This cannot prevent accidents from use of an explosive or a flammable substance.

Temperature setting range and functions

The unit has dual overheat preventive functions. One function is included in the controller and has been set at the time of factory shipping to automatically activate at the temperature 6°C higher than the set temperature of the temperature controller (The heater repeats ON/OFF at a temperature 6°C higher than the setting.)

The other function is integrated with the controller and is set by operating the keys on the controller.



This setting adds the second overheat prevention function.

The temperature setting range of the overheat preventive device integrated with the controller is from 0°C to 105°C.

If the temperature in the bath keeps rising above the controller set temperature and reaches the set temperature of the overheat preventive device, the circuit will be shut off, Er 19 will blink on the controller screen, and the buzzer continues sounding.

Once this overheat preventive device is activated, it holds that status until power is reset and Er19 will not be released.

How to set a temperature

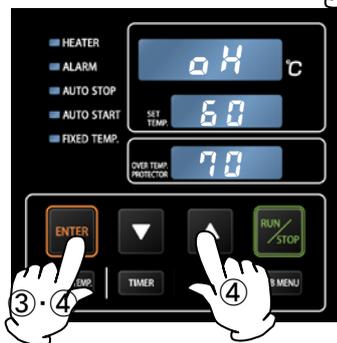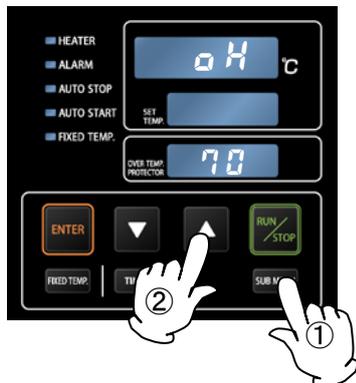

1. Turning power on (Turn the ELB ON)

When you turn power on, the initial values will be displayed for about four seconds, the screen will change to the initial setting screen and each display shows the current temperature in the bath, the operation mode characters, and the overheat prevention set temperature.

2. Setting the overheat prevention temperature

- ⑤ Press the **Sub menu** key.
- ⑥ Press the **▼▲** keys to select the overheat prevention setting characters **OH** on the measured temperature display.
- ⑦ Pressing the **Enter** key will make the current set temperature blink on the set temperature display.

Caution : Normally, set a temperature higher by 10°C or more than the set temperature on the controller to prevent a malfunction. However, please set it at a temperature that is 15°C or more higher when you drive the defrosting.

- ⑧ When you have set a temperature you want with the **▼▲** keys, press the **Enter** key to complete setting.

⚠ Caution


- ③ Rough guidelines for the set temperature are “the highest temperature possible for the unit +10°C” or “set temperature +10°C” and if malfunctions occur at these settings, add about 5°C to the setting.
- ④ The temperature setting range of the overheat preventive device is from 0°C to 135°C. Be sure to set the overheat prevention threshold temperature. Otherwise, devices may not operate properly, the overheat preventive device may activate in the middle of increase of the temperature in the bath, or a fire or other unexpected accidents may result.

The temperature is set at 90°C at factory shipping.

4-2. Operating procedures (upper stage)

Upper stage bath Operating procedures (fixed value operation)

How to conduct fixed value operation



1. Turning power on (Turn ELB ON)

When you turn power on, the software version will be displayed for about four seconds, the screen will change to the initial setting screen and each display shows the current temperature in the bath, the operation mode characters, and the overheat prevention set temperature.

- Measured temperature display : Displays the current temperature in the bath
- Set temperature display : Displays the operation mode characters
- Overheat prevention set temperature display : Displays the set temperature of the overheat prevention device

See P.19 for operation mode characters.



2. Selecting an operation mode

Press the **Fixed temp** key to display fixed value operation on the set temperature display.


Display Fix **F.11**.

3. Setting a temperature

① Press the **Fixed temp** key again.

The characters SV **50** that indicate temperature setting will appear on the measured temperature display, the current set temperature blinks on the set temperature display, and the fixed value operation lamp blinks.

② Set the temperature you want with the **▼▲** keys.

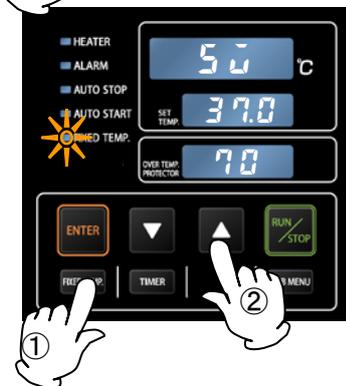

4. Starting operation

Press the **Start/Stop** key for about one second. Operation starts and the fixed value operation lamp will change its status from blinking to on.

5. Stopping operation

Press the **Start/Stop** key for about one second. The fixed value operation lamp will go off and the screen switches to the initial setting screen.



When you want to correct settings or confirm settings

If you made a mistake in setting or when you want to check the setting you have made, press the **Fixed temp** key again and make settings again.

If you want to change the set temperature during operation, press the **Fixed temp** key to enter the setting mode and change the temperature. After change, press the **Enter** key to complete change.

4-2. Operating procedures (upper stage)

Upper stage bath Operating procedures (Quick auto stop operation)

How to perform quick auto stop operation



This operation is used when you “want to stop current fixed value operation automatically after several hours”. Quick auto stop operation allows setting the auto stop timer during operation.

1. Setting a time until stop during fixed value operation

Make sure that the fixed value operation lamp is on to indicate fixed value operation is in session.

Press the **Timer** key.

The characters tim **E n** that indicate the timer appears on the measured temperature display and the current set time blinks on the set temperature display.

Set a time you want with the **▼▲** keys.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.



2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Start the timer operation when the fixed value operation lamp and the auto stop lamp are on.

Timer operation starts when the **Start/Stop** key is pressed.

Stopping and finishing timer operation

Timer operation will stop automatically at the set time.

The buzzer sounds for five seconds to indicate the timer has stopped. At this time, the characters End **End** that indicate operation complete are displayed on the set temperature display with the fixed value operation lamp and the auto stop lamp are on. Press the **Start/Stop** key for about one second to finish the timer operation mode. The screen will switch to the initial setting screen.


When you want to correct the set temperature, set time, or to confirm settings

When you want to change the set temperature during operation, press the **Fixed temp** key to enter the setting mode and change the temperature. After change, press the **Enter** key to complete change. If you want to change the set time during operation, press the **Timer** key to enter the setting mode and change the time. Note however, that you need to set a time calculated by adding the passed time to the time to add. After change, press the **Start/Stop** key to complete change. You can display the set temperature, the operation mode, and the remaining time on the set temperature display by pressing the **▼** key.

4-2. Operating procedures (upper stage)

Upper stage bath Operating procedures (auto stop operation)

How to perform auto stop operation

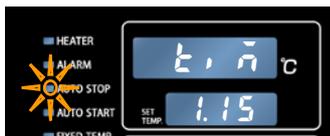

This operation mode is used when “you want to stop fixed value operation automatically after set time since the start”.

1. Setting a stop time


- ① Press the **Timer** key when the initial screen is displayed.
- ② The timer mode used in the previous session will be displayed on the set temperature display. Pressing the **Timer** key again to make a timer mode blink. Press the **Timer** key again to blink the next timer mode. Select the characters Astp **ASTP** that indicate auto stop operation and press the **Enter** key.

The characters Sv **5.0** that indicate temperature set appear on the set temperature display and the auto stop lamp will blink.

- ③ Press the **▼▲** keys to set the temperature you want.
- ④ Press the **Enter** key. The characters tim **1.15** that indicate the timer on the measured temperature display and the current set time will blink on the set temperature display.
- ⑤ Press the **▼▲** keys to set the time you want.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.

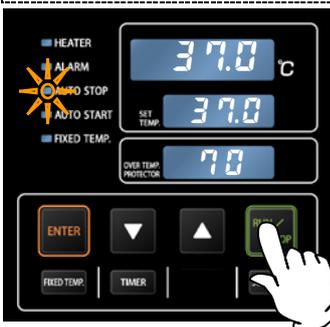

2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Timer operation will start with the auto stop lamp on.

Timer starts when the temperature in the bath (measured temperature) reaches the set temperature.

4-2. Operating procedures (upper stage)

Upper stage bath Operating procedures (auto stop operation)



3. Stopping and finishing timer operation

Timer operation will stop automatically at the set time.

The buzzer sounds for five seconds to indicate that the timer has stopped. At this time, the characters End End that indicate operation complete are displayed on the set temperature display with the fixed value operation lamp and the auto stop lamp are on. Press the Start/Stop key for about one second to finish the timer operation mode. The screen will switch to the initial setting screen.

When you want to correct the set temperature, set time, or to confirm settings

If you want to change the set temperature or the set time during operation, press the Timer key, set a temperature or a time for auto stop operation with the ▼▲ keys, and then press the Enter key.

Note however, that when you change the setting you need to set a time calculated by adding the passed time to the time to add.

You can press the ▼ key during operation to display the set temperature, the operation mode, and the remaining time on the set temperature display.

The remaining time display 1.30 indicates counting-down while the dots are blinking and waiting state while the dots stay on (temperature is increasing or decreasing toward the set temperature) and the timer count is stopped.

4-2. Operating procedures (upper stage)

Upper stage bath Operating procedures (auto start operation)

How to perform auto stat operation



Used for "Timing but not running after starting, and entering fixed value operation only after timing arrives." (Delayed operation)

1. Setting a startp time

- ① Press the **Timer** key when the initial screen is displayed.
- ② The timer mode used in the previous session will be displayed on the set temperature display. Pressing the **Timer** key again to make a timer mode blink. Press the **Timer** key again to blink the next timer mode. Select the characters Astr **Astr** that indicate auto start fixed value running and press the **Enter** key.

The characters Sv **50** that indicate temperature set appear on the set temperature display and the auto start lamp will blink.

- ③ Press the **▼▲** keys to set the temperature you want.
- ④ Press the **Enter** key. The characters tim **t. n** that indicate the timer on the measured temperature display and the current set time and autostarat lamp will blink on the set temperature display.
- ⑤ Press the **▼▲** keys to set the time you want.

About the timer function

The maximum timer setting possible is 999 hours 50 minutes. You can set a time in the unit of minutes up to 99 hours 59 minutes. The setting unit will be 10 minutes for a time of 100 hours or longer. You can change a set time quickly to the time you want by keeping the **▼▲** keys pressed. To fine adjust a time, repeat pressing the **▼▲** key for each digit.

2. Starting timer operation

When you have set a time you want, press the **Start/Stop** key for about one second.

Timer operation will start with the auto start lamp on



4-2. Operating procedures (upper stage)

Upper stage bath Operating procedures (auto start operation)



3. Stopping and finishing timer operation

Operation will start automatically when the set time comes.

Press the **Start/Stop** key for about one second to stop or finish operation. The screen switches to the initial setting screen.

When you want to correct the set temperature, set time, or to confirm settings

If you want to change the set temperature or the set time during operation, press the **Timer** key, set a temperature or a time for auto start fixed value running with the **▼▲** keys, and then press the **Enter** key.

Note however, that when you change the setting you need to set a time calculated by adding the passed time to the time to add.

You can press the **▼** key during operation to display the set temperature, the operation mode, and the remaining time on the set temperature display.

Note that you cannot change them if you have started operation after the auto start time has passed. In this case, stop operation once with the **Start/Start** key and resume setting from the start.

4-1. Operating procedures (upper stage)


Upper stage bath Useful functions (calibration offset function)

Using the calibration offset function

The calibration offset function compensates any difference between the target in-bath temperature and the control temperature of the controller (sensor temperature). You can apply parallel compensation to the plus or minus side over the entire temperature range of the unit.

You can set/cancel this function with the **Sub menu** key.

The offset is set at “0” at the time of factory shipping.

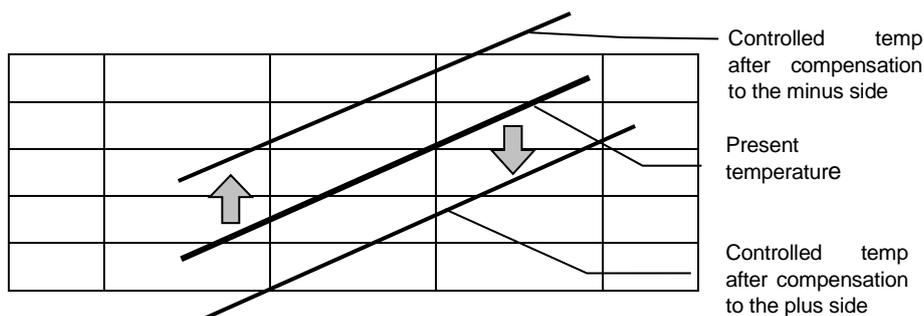

- ① Start operation at the target set temperature and check the in-bath temperature (sample temperature) on a temperature recorder when the temperature is stable.
- ② Check the difference between the set temperature and the in-bath temperature (sample temperature).
- ③ Press the **Sub menu** key and select the character cAL **cAL** that mean calibration offset with the **▼▲** keys and then press the **Enter** key.
- ④ Enter the difference between the set temperature and the in-bath temperature with the **▼▲** keys and press the **Enter** key longer to finish setting.

※ You can set an offset compensation temperature within the range from +99°C to -99°C.

Setting to the - side will decrease the temperature on the measured temp indicator by the compensated temperature and the in-bath temperature will increase by that amount accordingly.

Setting to the + side will increase the temperature on the measured temp indicator by the compensated temperature and the in-bath temperature will decrease by that amount accordingly.

※ Inputting a too large compensation value may cause the actual temperature greatly deviate from the displayed temperature and may be dangerous. So please consult the nearest sales office beforehand.

※ The unit has a two-point compensation function that adjusts offset for the lower temperature region and the high temperature region in addition to the calibration offset function and adjusting temperatures have been set at the time of factory shipping.

※ When validating the temperature indicator, first consult with your nearest sales office or the customer support center.

4-2. Operating procedures (upper stage)

Upper stage bath Useful functions (lock function)

Using the lock function

This function is used to lock the operating status you have set.

This function is set to “off” at factory shipping.



You can set or release this function with the **Sub menu** key.

④ Press the **Sub menu** key, select the characters Lock **Lock** that indicate the setting lock with the **▼▲** keys, and then press the **Enter** key.

⑤ "OFF" will appear on the set temperature display. You can lock the settings by setting to "ON" with the **▲** key.

⑥ To release lock, press the **Sub menu** key, select the characters Lock **Lock** that indicate the setting lock with the **▼▲** keys, and then press the **Enter** key.



Select "OFF" with the **▼** key and then press the **Enter** key to release.



※While the lock function is "ON", any keys other than the **Start/Stop** key and the **Sub menu** key are locked.

5. Handling precautions

Warning

1. About non-supported substances

-  Never use an explosive substance, a flammable substance, or those that contain such substances for the unit. Otherwise, an explosion or a fire may result.
See "13. List of dangerous materials" on page 61.

2. Ban of use/measures in an abnormality

-  何 If this unit should generate a smoke or a strange odor for unknown reason, immediately turn the ELB of the main unit and the power off and ask your dealer or one of our sales offices for inspection. Leaving the unit in such a state may cause a fire or an electrical shock. Never attempt to repair the unit by yourself, which poses a danger.

Caution

1. Never climb on the unit.

-  Never climb on the unit. The unit may topple over or be damaged and a personal injury or a malfunction may result.

2. Do not place an object on the unit.

-  Do not put an object on the unit. It may fall off and may cause a personal injury. Also, do not put a piece of paper or other objects that are highly combustible around the unit.

3. When a thunder is heard.

-  When a thunder is heard, immediately turn the unit and the power supply off.
Leaving them as it is may cause the control circuit of the unit malfunction or a fire or an electric shock from a lightning.

4. When opening/closing a door.

-  When opening/closing a door, do not put your hand or face close to the area (space) where the door is movable. The door may hit your hand or face and cause an injury.

5. Do not operate the unit with its door left open.

-  Operating the unit with its door open will prevent proper temperature control causing the heater overheat to a dangerous level. Be sure to close the door while operating the unit.

6. Ban on use of a corrosive specimen

-  Although SUS304 stainless steel is used for the inside of the bath, note that it might corrode with a strong acid. Door packing are made of vinyl chloride rubber. Note that it may corrode with acids, alkalis, oils, or halogen based solvents.

5. Handling precautions



Caution

7. Use the unit at an appropriate temperature.



Operating temperature range: Upper stage bath : Room temperature +5°C~80°C; lower stage bath : 4°C~50°C.

Never operate the unit at a temperature outside the operating temperature range.

8. Assure sufficient ventilation of the unit.



Do not operate the unit with ventilation ports at the front, sides, and back of the unit covered. Internal temperature of the unit will rise degrading the performance and may cause an accident, a malfunction, or a fire.

9. Take care not to allow liquid splash on the unit.



Take care not to allow liquid splash on the unit. In particular, take care not to allow liquid entering into the ventilation ports at the front, sides, and back of the unit. Stop operating the unit if liquid should splash on the unit. Otherwise, an accident, a malfunction, an electric shock, or a fire may result.

10. Do not drop a metal piece inside the unit.



Do not drop a clip, a staple, a screw, or other metal pieces inside the unit.

Stop operating the unit if a metal piece is dropped inside the unit.

Otherwise, an accident, a malfunction, an electric shock, or a fire may result.

11. About placement of shelf boards and specimens.



Place shelf boards and specimens correctly according to the "Installation method and precautions" on page 8. Incorrect placement will prevent sufficient performance from exerting and an accident or a malfunction may result.

12. Never attempt to perform works not specified in this instruction manual.



Never attempt to perform works not specified in this instruction manual. Otherwise, an unexpected accident may result.

13. About recovery from a power failure.



When the unit stopped operation due to a power failure and power is supplied again, the unit automatically recovers to the status immediately before the failure and resumes operation.

We recommend turning power off because it is dangerous if the unit restarts suddenly when the power recovers from the power failure.

14. About vibrations.



There is a freezer on the lower stage of the unit and it causes some vibrations. Do not use the unit for tests that shall avoid vibrations including protein crystallization.

(Use our low temperature incubator IN602N when you needs a low vibration unit.)

6. Maintenance

Daily inspection/maintenance

Warning


- Be sure to remove the power cord before inspection or maintenance unless necessary.
- Start working after the unit temperature has returned to the normal temperature.
- Never attempt to disassemble devices.

Caution

- Wipe off any dirt with a well wrung out soft cloth. Never use benzene, thinner, or scorching powder or rub with a hard brush. Otherwise, deformation, deterioration, or discoloration may result.


Monthly

- Inspect the function of the ELB.
 - ˘ Connect the power cord and conduct a test while it is activated.
 - ˘ First turn the ELB “off”.
 - ˘ Then turn it “on” and push the test button of the ELB with a pointed object such as a ball point pen and it is normal if it is turned off.

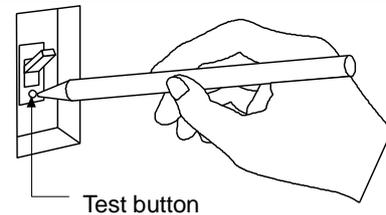

- Check the operation of the overheat preventive device.
 - ˘ After performing fixed value operation at an appropriate set temperature, set the operation temperature of the independent overheat preventive device to a temperature lower by several degrees (about 5°C).
 - ˘ If the ELB is normal, the heater circuit will be shut off after several seconds and the “Alarm” sign and Er19 will come on and the alarm buzzer sounds at the same time.
- Clean the fins of the condenser.

Remove the grill of the unit and remove dusts on the condenser fins using a vacuum cleaner.

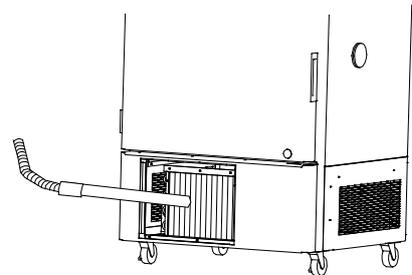

Caution

Take care not to crush the fins when cleaning.

※ Be sure to perform operation check for the ELB and the overheat preventive device above before a continuous operation for a long time or unmanned operation during nighttime.

Maintenance of the internal bath

Stop operation and turn the ELB “off”. Remove the power cord and the distribution panel from the outlets. Check the internal temperature and then remove the shelf boards and the shelf pegs.

The internal bath, shelf boards, shelf pegs are made of SUS304 stainless steel and the inner door employs reinforced glass. Use a cloth soaked in cleaning alcohol, wipe it thoroughly, and then wipe lightly with a dry cloth for cleaning. Never use an acid cleaner, an alkaline cleaner, oils, or an organic solvent, which will cause corrosion or damages.



Take special care for injury with keen protruding parts inside the internal bath, on the shelf boards, and the shelf pillars. Be sure to wear gloves and never handle them with bare hands to avoid injury.

7. When the unit is not to be used for a long time or when disposing

 Warning	 Caution
When you are not going to use the unit for a long time ● Turn power off and remove the power cord.	When disposing ● Do not leave the unit where children may play around. ● Remove all driving assemblies. ● The unit uses CFC's substitute. Ask the professional company for its disposal.

Notes about disposition

Always pay attention to the preservation of the global environment.

- We highly recommend taking the unit apart as far as possible for separation or recycling to contribute to the preservation of the global environment. Major components and materials for the unit are as follows:

Names of major components	Material
Major components of the exterior	
Exterior	Electro galvanized steel plate, melamine resin baking finish
Interior	SUS304 stainless steel plate
Heat insulator	Styrene foam, glass wool
Sealant	Polyester film
Major components of the electric system	
Switches and relays	Resin, copper, other composite products
Operation panel	Alkyl benzene sulfide (ABS)
Board	Glass fiber, other composite products
Heater	Iron chrome wire
Power cord	Synthesized rubber covering, composite products of copper, nickel, etc.
Sealant	Resin based material
Sensor (Pt&K double sensor)	SUS304 stainless steel, other
Freon	R134A ※1

- ※1 Freon is specified as the class 1 specific product in Freon recovery and destruction law. Emission of Freon into atmosphere without rational reasons is prohibited by law. When discarding the product, its Freon must be collected.

8. When a trouble occurs


Safety devices and error codes

The unit has a self diagnostic function integrated in the controller.

The table below shows the possible causes for an activation of a safety device and solutions.

[Error codes]

When an operational abnormality or a unit malfunction occurs, operation will stop, the alarm lamp on the operation panel comes on, an error code appears, and the alarm buzzer sounds.

Safety device	Symptom	Causes and countermeasures
Sensor error detected	Alarm lamp on  indication	<ul style="list-style-type: none"> Disconnection or a malfunction of the temperature sensor Contact the general customer service center.
SSR short-circuit detected	Alarm lamp on  indication	<ul style="list-style-type: none"> SSR short-circuit Contact the general customer service center.
Heater disconnection detected	Alarm lamp on  indication	<ul style="list-style-type: none"> Heater disconnection Contact the general customer service center.
Malfunction of memory	Alarm lamp on  indication	<ul style="list-style-type: none"> Abnormality in settings in memory Contact the general customer service center.
Internal communication error	Alarm lamp on  indication	<ul style="list-style-type: none"> Error in internal communication or in the temperature input circuit. Contact the general customer service center.
Abnormal rise of temperature	Alarm lamp on  indication	<ul style="list-style-type: none"> Activation of the overheat preventive device Reset the power supply once and then check the temperature in the bath and the set temperature of the overheat preventive device. If the unit does not recover, contact the general customer service center.
Compressor failure	Alarm lamp on  indication	<ul style="list-style-type: none"> Compressor failure Compressor thermal protection, power off and stop for 10 minutes before running again. If the unit does not recover, contact the general customer service center.
Abnormal measured temperature	Alarm lamp on  indication	<ul style="list-style-type: none"> When the measured temperature is outside the display range. Contact the general customer service center.

8. When a trouble occurs

Safety units and error codes

In the following cases

Symptom	Check
The ELB will not become active even if power is turned on.	<ul style="list-style-type: none"> ● If the power plug is connected to the receptacle correctly. ● If a power failure has occurred.
The alarm lamp comes on.	<ul style="list-style-type: none"> ● Check error codes. Check the meaning of the error code in "Safety devices and error codes" on P54.
Temperature will not increase.	<ul style="list-style-type: none"> ● If the set temperature is lower than the internal temperature. ● If supply voltage has been low. ● If the environmental temperature is low. ● If cooling load in the bath is large.
Temperature will not decrease.	<ul style="list-style-type: none"> ● If the set temperature is higher than the internal temperature. ● If supply voltage has been low. ● If the environmental temperature is high. ● If heat load in the bath is large. ● If the ventilation ports and around them are covered.
Temperature fluctuates during operation.	<ul style="list-style-type: none"> ● If set temperature is appropriate. ● If supply voltage has been low. ● If changes of the environmental temperature are large. ● If load in the bath is large.
Display temperature is not in accordance with measured temperature	<ul style="list-style-type: none"> ● If the set value of offset is not 0, please set as 0. Confirm the set value on P36 Lower stage bath Useful functions (calibration offset function) or P49 Upper stage bath Useful functions (calibration offset function)

If a power failure occurs

During operation, the operation is stopped due to power failure. When the power is supplied again, the product will be automatically restored to the operating state before power failure.

When it is not necessary to use automatic recovery for reoperation after power failure, please disconnect the leakage protector switch.

- ◆ When the symptom does not correspond to any of the above, immediately turn the ELB on the main unit off, remove the power plug out of the power supply and contact your dealer, one of our sales offices, or our general customer service center.

9. After sales service and warranty

When requesting a repair

When requesting a repair

If any trouble occurs, immediately stop operation, turn the ELB off, pull out the power plug and contact your dealer or our sales office.

Information necessary for requesting a repair

- Model name of the product
 - Serial number
 - Date (y/m/d) of purchase
 - Description of trouble (as in detail as possible)
- } See the warranty card or the nameplate on the unit.
} See the section “3. Names and functions of parts” on page 11.

Be sure to indicate the warranty card to our service representative.

Warranty card (attached separately)

- Your dealer or one of our sales offices will hand you a warranty card. Please fill necessary data such as “dealer name, date of purchase, etc” and store at a safe place.
- Warranty period is one full year from the date of purchase. Repair service for free is available according to the conditions written on the warranty card.
- For repairs after the warranty period consult your dealer or one of our sales offices. Paid repair service is available on your request when the product’s functionality can be maintained by repair.

Minimum holding period of repair parts

The minimum holding period of repair parts for this product is seven years after end of production.


Repair parts here refer to parts necessary for maintaining performance of the product.

10. Specifications

Model		INC822C	
		Upper stage bath	Lower stage bath
System		Air jacket natural convection	Forced blow circulation
Performance	Operating temp range	Room temperature +5~80°C	-10°C~60°C
	Temp adjusting precision	±0.5°C (at37°C)	±0.5°C
	Temp distribution precision	±1.0°C (at37°C)	±1.0°C (at 37°C) ±1.5°C (at other operating temp.)
Configuration	Interior	SUS304 stainless steel plate	
	Exterior	Electro galvanized steel plate, SECC	
	Heat insulator	Glass wool	Styrene foam
	Heater	Iron-chrome wire heater	
		400W	550W
	Blower fan	—	Axial fan
	Freezer	—	Air-cooled hermetic compressor :158W
	Cooling medium	—	R134A
	Defrosting function	—	Hot gas bypass system
	Cable ports	φ 30 (right side of exterior)	φ 50 (right side of exterior)
	Air supply port	Interior bottom	—
Discharge port	φ 30x2 (ceiling)	—	
Control assembly	Controller		Model VS6
	Temp control/heater control		PID system/SSR control
	Sensor	Temp control	Pt100Ω
		Overheat prevention in bath	K-thermocouple
Safety devices		Self diagnostic function (temp sensor malfunction, heater disconnection, SSR short-circuit, automatic overheat prevention (controller integrated)), key lock, over current ELB, overheat preventive device in bath.	
Standard	External dimensions ※1 (W x D x H)	710 × 656 × 1792 mm	
	Internal dimensions (W x D x H)	600 × 530 × 500 mm	600 × 477 × 500 mm
	Power supply	AC220V 50Hz 8A	
	Weight	Approx. 160 kg (during drying)	
	Number of shelf stages	2	3
	Withstand load of shelf board	Approx. 15 kg/each	
	Shelf peg pitch	13 stages: 30 mm	13 stages: 30 mm
Accessories	Shelf board : Stainless steel punched metal 3 + 2=5 Shelf peg : shelf boards x 5 x 2=10 pieces Instruction manual, warranty card, door keys x 2		

※1 External dimensions do not include protruding parts.

11. Wiring diagram

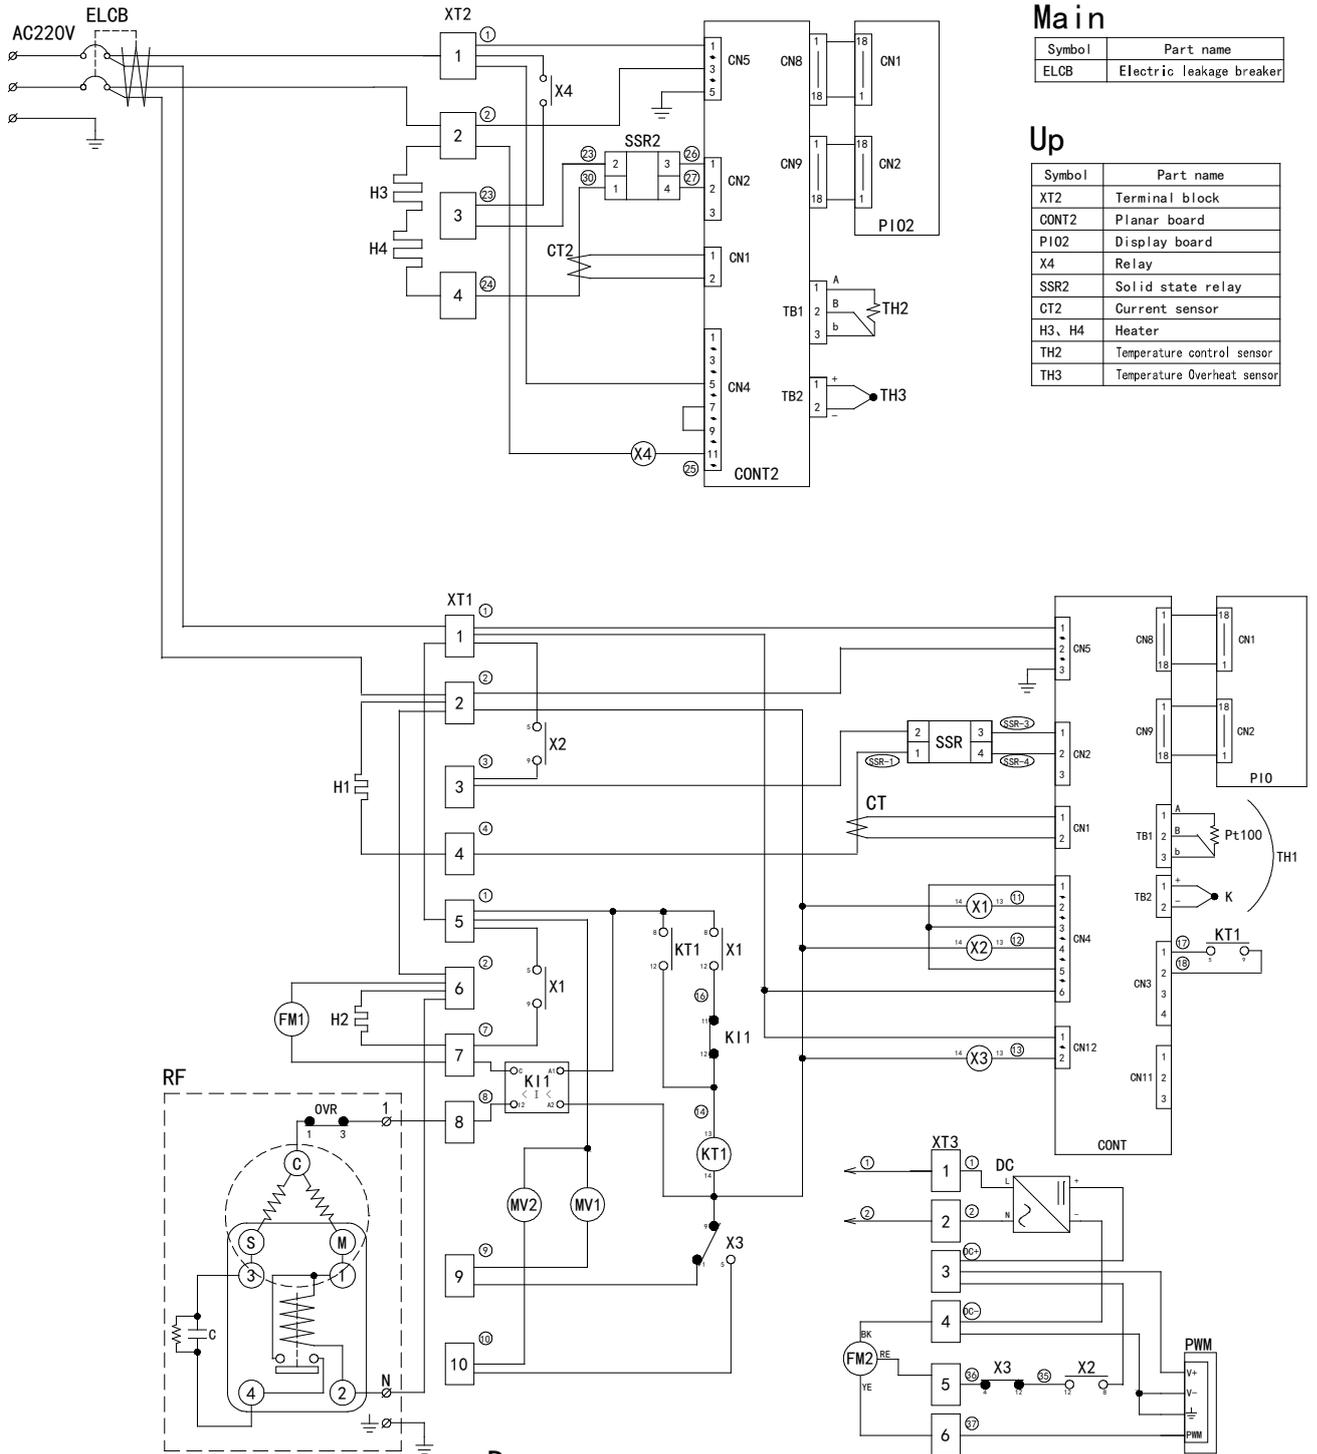

Main

Symbol	Part name
ELCB	Electric leakage breaker

Up

Symbol	Part name
XT2	Terminal block
CONT2	Planar board
PI02	Display board
X4	Relay
SSR2	Solid state relay
CT2	Current sensor
H3, H4	Heater
TH2	Temperature control sensor
TH3	Temperature Overheat sensor

Down

Symbol	Part name	Symbol	Part name
XT1	Terminal block	FM2	Fan motor (inside)
CONT1	Planar board	MV1	Solenoid valve (return pipe)
PI01	Display board	MV2	Solenoid valve (defrost)
X1	Relay (freezer)	K11	Current relay
X2	Relay (internal heater)	KT1	Time relay
X3	Relay (defrost)	TH1	Temperature sensor (double)
SSR1	Solid state relay	Pt100	Temperature control sensor
CT1	Current sensor	K	Temperature Overheat sensor
H1	Heater (inside)	RF	Freezer
H2	Heater (door)	OVR	Over power relay
FM1	Fan motor (freezer)	C	Operation capacitor
XT3	Terminal block	PWM	Speed control module
DC	DC Power		

12. Replacement part table

Symbol	Part name	Code No.	Specification	Maker
CONT1-2	Planar board	B011401053	VS6	Yamato
PIO1-2	Display board	B011402007	VS mode	Yamato
SSR1-2	Solid state relay	A011006023	KS15/D-38Z25-L	Yamato
KI1	Current relay	A011008004	K8DT-AW2CA	OMRON
TH1	Temperature sensor (double)	A010502052	T0304_03-78 PT and K	Yamato
KT1	Current relay	A011004006	H3Y-2 AC200-230V 30s	OMRON
X1-3	Relay	A011002007	HF13F/A220Z1D	OMRON
CT1-2	Current relay	B010509001	CTL-6-S-4	OMRON
XT1	Terminal block	B011301024	MKH-250ABC-10P	Yamato
	Power cable	A011209001	PSE JET VCTF 3x2.0mm2	Yamato
ELCB	Electric leakage breaker	A010410007	BV-DN IP+N 10A 30mA	MITSUBISHI
FM2	Fan motor	A080104062	HE30H420A22BF	Yamato
MV1	Solenoid valve	A031800001	1028/2	Yamato
MV2	Solenoid valve	A031800002	1068/3	Yamato
FM1	Fan motor	A011603020	iQC3612-010105-C02	Yamato
	Desiccator	A031502001	1/4"	Yamato
RF1	Freezer	A030200034	EMT45HDR 220-240V 50Hz	Yamato
H1	Heater	B080504011	550W/220V	Yamato
H2	Heater	B080504009	16W/220V	Yamato
	Evaporimeter	H050301009	IN612C_01_06_02	Yamato
	Capillary	SJA04177	φ0.75×φ3×400 mm	Yamato
	Capillary	SJA04178	φ1.0×φ2.2×1800 mm	Yamato
XT2	Terminal block	B011301012	MKH-250ABC-4P	Yamato
X4	Relay	A011002002	HF116F-2/220AL1HSTFW	OMRON
H3-4	Heater	B080504003	100V,200W	Yamato
TH2	Temperature sensor	H050101001	Pt100Ω(T0304.01-02)	Yamato
TH3	Temperature sensor	H010101001	φ3.2*55*2000	Yamato
DC	DC POWER	A010801065	LRS-50-24	Yamato
PWM	PWM module	A020599002	PWM module	Yamato
XT3	Terminal block	B011301003	MKH-250ABC-6P	Yamato

13. List of dangerous materials



Never use an explosive substance a flammable substance or a substance containing them for this device.

Explosive substance	Explosive substance	① Nitroglycol, glycerine trinitrate, cellulose nitrate and other explosive nitrate esters
		② Trinitrobenzen, trinitrotoluene, picric acid and other explosive nitro compounds
		③ Acetyl hydroperoxide, methyl ethyl ketone peroxide, benzoyl peroxide and other organic peroxides
Flammable substances	Explosive substances	Metal "lithium", metal "potassium", metal "natrium", yellow phosphorus, phosphorus sulfide, red phosphorus, celluloids, calcium carbide (a.k.a, carbide), lime phosphide, magnesium powder, aluminum powder, metal powder other than magnesium and aluminum powder, sodium dithionous acid (a.k.a., hydrosulphite)
	Oxidizing substances	① Potassium chlorate, sodium chlorate, ammonium chlorate, and other chlorates
		② Potassium perchlorate, sodium perchlorate, ammonium perchlorate, and other perchlorates
		③ Potassium peroxide, sodium peroxide, barium peroxide, and other inorganic peroxides
		④ Potassium nitrate, sodium nitrate, ammonium nitrate, and other nitrates
		⑤ Sodium chlorite and other chlorites
		⑥ Calcium hypochlorite and other hypochlorites
	Flammable substances	① Ethyl ether, gasoline, acetaldehyde, propylene chloride, carbon disulfide, and other substances with ignition point at a degree 30 or more degrees below zero.
		② n-hexane, ethylene oxide, acetone, benzene, methyl ethyl ketone and other substances with ignition point between 30 degrees below zero and less than zero.
		③ Methanol, ethanol, xylene, pentyl acetate, (a.k.a.amyl acetate) and other substances with ignition point between zero and less than 30 degrees.
		④ Kerosene, light oil, terebinth oil, isopenthyl alcohol(a.k.a. isoamyl alcohol), acetic acid and other substances with ignition point between 30 degrees and less than 65 degrees.
Combustible gas	Hydrogen, acetylene, ethylene, methane, ethane, propane, butane and other gases combustible at 15°C at one air pressure.	

14. Standard installation manual

※Install the unit according to the items below. (Confirm optional or special specifications.)

Model	Serial number	Date	Inst. Manager(company name)	Inst. manager	Judge

No.	Item	Implementation method	TOC No.	Ref. column of manual	Judge	
Specifications						
1	Accessories	Check items based on the accessories column	10.	Specification column P.57		
2	Installation	<ul style="list-style-type: none"> Visual check of the environmental conditions Caution : Surrounding environment Securing a space 	2.	Before operating the unit on P.4 installation...		
Operation related matters						
1	Source voltage	<ul style="list-style-type: none"> Measure customer side voltage (at a distribution board and an outlet, etc.) with a tester. Measurement of an operating voltage (must meet the standard) Caution : Use a product that comply with the standard for installing to a plug or a breaker. 	2.	Before operating the unit <ul style="list-style-type: none"> Be sure to connect the earth... Connect the power supply to a dedicated outlet 10. Specifications <ul style="list-style-type: none"> Standard—power supply 	P.6 P.6 P.57	
2	Starting operation	<ul style="list-style-type: none"> Start operation Perform fixed value operation, auto stop operation, and auto start operation..	2.	Before use P.4~10 <ul style="list-style-type: none"> Installation method... 4.How to operate	Lower stage P.17~36 Upper stage P.37~49	
Description						
1	Description of operation	Explain operation of each part to the customer as per the instructions.	4.	Operating procedures <ul style="list-style-type: none"> Operating method 1.Safety precautions	P.17~49 P.1~13. List of dangerous substances	
2	Error codes	Explain error codes and how to release to the customer as per the instructions.	8.	When a trouble occurs <ul style="list-style-type: none"> ~9.After sales service and warranty 	P.54~56	
3	Maintenance and inspection	Explain operation of each part to the customer as per the instructions.	6.	Maintenance procedures <ul style="list-style-type: none"> Daily inspection/ maintenance 	P.52	
4	Matters to note on completion of installation	<ul style="list-style-type: none"> Note the installation date and the manager on the nameplate. Note necessary matters in the warranty card and hand it to the customer. Explain the after sales service route. 	9.	After sales service and warranty	P.56	

Responsibility

Please follow the instructions in this document when using this unit. Yamato Scientific has no responsibility for the accidents or breakdown of device if it is used with a failure to comply. Never conduct what this document forbids. Unexpected accidents or breakdown may result in.

Note

- ◆ The contents of this document may be changed in future without notice.
- ◆ Any books with missing pages or disorderly binding may be replaced.

Instruction Manual
Program Type Low Temperature Incubator/
Constant Temperature Incubator
Model INC822C

First edition Sep 10, 2025

Revised on Jan 04, 2026

YAMATO SCIENTIFIC CO., LTD.
Harumi Triton Square Y-36F, 1-8-11 Harumi,
Chuo-ku, Tokyo 104-6136, Japan
Tel : +81-3-5548-7122
Fax : +81-3-5548-0132
<https://www.yamato-scientific.com/>